

Integrating the Healthcare Enterprise



5

IHE Patient Care Device Technical Framework Supplement

10

Infusion Pump Event Communication (IPEC)

15

Trial Implementation

Date: August 12, 2011

Editor: John Rhoads

Email: pcd@ihe.net

20

Foreword

This is a supplement to the IHE Patient Care Device Technical Framework 1.0. Each supplement undergoes a process of public comment and trial implementation before being incorporated into the volumes of the Technical Frameworks.

25 This supplement is submitted for Trial Implementation as of August 12, 2011 and will be available for testing at subsequent IHE Connectathons. The supplement may be amended based on the results of testing. Following successful testing it will be incorporated into the Patient Care Device Technical Framework. Comments are invited and can be submitted at <http://www.ihe.net/pcd/pcdcomments.cfm> or by email to pcd@ihe.net.

30 This supplement describes changes to the existing technical framework documents and where indicated amends text by addition (**bold underline**) or removal (~~**bold strikethrough**~~), as well as addition of large new sections introduced by editor’s instructions to “add new text” or similar, which for readability are not bolded or underlined.

35 “Boxed” instructions like the sample below indicate to the Volume Editor how to integrate the relevant section(s) into the relevant Technical Framework volume:

General information about IHE can be found at: www.ihe.net

Information about the IHE Patient Care Device domain can be found at:
<http://www.ihe.net/Domains/index.cfm>

40 Information about the structure of IHE Technical Frameworks and Supplements can be found at:
<http://www.ihe.net/About/process.cfm> and <http://www.ihe.net/profiles/index.cfm>

The current version of the IHE Technical Framework can be found at:
http://www.ihe.net/Technical_Framework/index.cfm

45

CONTENTS

INTRODUCTION4

50 PROFILE ABSTRACT.....4

OPEN ISSUES AND QUESTIONS4

CLOSED ISSUES.....4

VOLUME 1 – CONTENT PROFILES.....5

1.7 HISTORY OF ANNUAL CHANGES5

1.N COPYRIGHT PERMISSION5

55 2.1 DEPENDENCIES AMONG INTEGRATION PROFILES5

 2.2.X *Infusion Pump Event Communication Integration Profile*5

X INFUSION PUMP EVENT COMMUNICATION (IPEC) INTEGRATION PROFILE7

X.1 ACTORS/TRANSACTIONS.....8

X.2 IPEC OPTIONS9

60 X.3 IPEC ACTOR GROUPINGS AND PROFILE INTERACTIONS10

X.4 INFUSION PUMP EVENT COMMUNICATION PROCESS FLOW.....10

 X.4.1 *Standard Use Cases*.....10

 X.4.1.1 Case IPEC-1: Communicate event data to EMR/EHR10

X.5 IPEC SECURITY CONSIDERATIONS11

65 **APPENDIX A ACTOR SUMMARY DEFINITIONS.....11**

APPENDIX B TRANSACTION SUMMARY DEFINITIONS.....11

GLOSSARY12

VOLUME 2 - TRANSACTIONS13

70 3.Y COMMUNICATE INFUSION EVENT DATA13

 3.Y.1 *Scope*.....13

 3.Y.2 *Use Case Roles*13

 3.Y.3 *Referenced Standard*.....13

 3.Y.4 *Interaction Diagram*14

 3.Y.4.1 Communicate Infusion Event Data.....14

 3.Y.4.1.1 Trigger Events.....14

 3.Y.4.1.2 Message Semantics14

 3.Y.4.1.3 Expected Actions15

75 **APPENDIX X INFUSION PUMP EVENTS.....15**

X.1 BASIC INFUSION EVENTS.....15

80 X.1.1 *Event Message – PCD-10 Communicate Infusion Event Data*.....17

X.1.2 *Infusion Pump Events*18

 X.1.2.1 Infusion Event Parameters.....18

 X.1.2.2 Infusion Event Sample Messages34

85

Introduction

90 This Supplement adds sections to the PCD Technical Framework Volume 1 describing the content associated with communicating Infusion Pump device events, and to Volume 2 describing data content and constraints.

Profile Abstract

95 The Infusion Pump Event Communication (IPEC) Profile specifies methods for communicating significant clinical and technical events from a Patient Care Device such as infusion pump to an information system which may present it to a clinical user, acts on it in some way or records it. The information is communicated in a data format similar to that of Device Enterprise Communications (DEC) Profile, but differs in that DEC is mainly used for sampled physiological and technical data at timed, equal intervals, while IPEC is used to communicate significant occurrences which happen at unscheduled times. Infusion Pump Event
100 Communications is also related to Alarm Communications Management (ACM) Profile, except that ACM is designed for physiological alarms and technical alerts to a human actor via portable devices, where IPEC is designed for system-to-system communication for automated recording or tracking occurrences which do not necessarily require urgent attention from a person.

Open Issues and Questions

- 105 • For future considerations:
- Include a unique event identifier in order to help in associating related events (delivery starts and delivery stops). Since there are many different use cases in pump operation, it may be that this is not feasible. Further analysis is needed. In the
110 meantime this can be accomplished using patient, device and order identifiers that are present in the PCD-10 message.
 - Support for subscription option for event messages.
 - Harmonize Patient ID Change event with the Point of Care Identity Management (PCIM) work group.
 - Determine Containment level for optional events.
 - 115 • ORU^Rxx trigger event number will be assigned at a later time.
 - Possible alignment with the Pharmacy domain through the use of the RAS^O17 message instead of ORU^Rxx

Closed Issues

120

Volume 1 – Content Profiles

1.7 History of Annual Changes

Add the following bullet to the end of the bullet list in section 1.7

- Added the Infusion Pump Event Communication profile which specifies the transmission of event information from infusion pumps to other information systems.

125

1.n Copyright Permission

<No new information>

2.1 Dependencies among Integration Profiles

Add the following to Table 2-1

Integration Profile	Depends On	Dependency Type	Purpose
Infusion Pump Event Communication	Consistent Time	Each actor implementing IPEC shall be grouped with the Time Client Actor	Required for consistent time-stamping of event data.

130

Add the following section to section 2.2

2.2.X Infusion Pump Event Communication Integration Profile

135

This document introduces a new profile - Infusion Pump Event Communication. This profile is based on the general observation reporting in Device Enterprise Communication (DEC) Profile. Infusion Pump Event Communication uses the same general form of interactions among Device Observation Reporter and Device Observation Consumer actors.

The principal intended uses of IHE Device Enterprise Communication in acute care are to communicate device data to enterprise information systems for:

140

- Reporting, charting and trending physiological data to assist clinicians in tracking the patients physiological state for situational awareness and care planning
- Near-real-time response to clinically or technically actionable events and situations
- Provision of information for an archival record of device observations, possibly including events, that are clinical, technical, or both

145 Device Enterprise Communications (DEC) is chiefly designed for the first goal listed based on periodic observation reporting, but has always provided for episodic and event reporting as a subtype of general event reporting.

This Infusion Pump Event Communication Integration Profile is designed to address the second goal of reporting events, specifically infusion pumps events. It defines a means for communicating significant events in medication administration by infusion pumps.

150

<i>Add section X</i>

X Infusion Pump Event Communication (IPEC) Integration Profile

155 This document introduces a new profile - Infusion Pump Event Communication. This profile is based on the general observation reporting in Device Enterprise Communication (DEC) Profile. Infusion Pump Event Communication uses the same general form of interactions among Device Observation Reporter and Device Observation Consumer actors.

The principal intended uses of IHE Device Enterprise Communication in acute care are to communicate device data to enterprise information systems for:

- 160 • Reporting, charting and trending physiological data to assist clinicians in tracking the patients physiological state for situational awareness and care planning
- Near-real-time response to clinically or technically actionable events and situations
- Provision of information for an archival record of device observations, possibly including events, that are clinical, technical, or both

165 Device Enterprise Communications (DEC) is chiefly designed for the first goal listed based on periodic observation reporting, but has always provided for episodic and event reporting as a subtype of general event reporting.

This Infusion Pump Event Communication Integration Profile is designed to address the second goal of reporting events, specifically infusion pumps events. It defines a means for communicating significant events in medication administration by infusion pumps.

170

Events in Medical Device Communications

175 An event, in the context of medical device communications, is an occurrence about which it is desired to communicate information between devices and information systems. Events are communicated as soon after their occurrence as is technically feasible, in contrast to other observation reporting in from devices to information systems which capture the trend of continuously-varying physiological characteristics indicating the patient's clinical status by communicating observations an even time interval characteristics. These characteristics are usually then displayed to clinical users in a spreadsheet-like grid or on a trend graph.

180 One special sort of event is an episodic measurement, that is, one that is not automatically initiated on a regular, timed basis, such as a spot blood pressure cuff reading, or a non-continuous cardiac output measurement. These are initiated manually and the receiving information system has no foreknowledge of when they will occur.

185 Another special case is an alert or alarm, where the key outcome of the event is meant to be some action by a person. The IHE PCD Alarm Communication Management (ACM) profile is focused on the human notification aspect of this.

Relation of Infusion Pump Event Communication to Alarm Communication Management Profile

190 Alarm Communication Management has provided expanded formats with additional attributes for alarms, with emphasis on transmitting the information to specific individuals who need to be notified at the point of care via portable devices. This has been supplemented by Waveform Communication profiling work which allows associating waveform data with an alarm.

For purposes of this discussion, a distinction is made between events and alarms.


- 195 • Events are operational milestones and key parameter changes. For example, during normal execution of an infusion therapy, non-alarm conditions such as start of delivery, change of rate, switchover from piggyback to primary drug, completion of delivery, transition to KVO, etc. are important to full recording or state awareness for the therapeutic process.
- 200 • Alarms are a subset of events which are intended to engage immediate response from the clinician, and are handled in the Alarm Communication Management profile.

Clinical information systems must communicate, for real-time high-reliability review and action, and record for documentation purposes:

- 205 • Exception Events – physiological or technical, which may indicate conditions either in the patient or in the equipment in use by those caring for the patient, which need attention at stated levels of urgency. These include alarms, appropriately processed for human notification using the Alarm Communication Management profile, but may in addition need to be communicated to information systems for other purposes than immediate notification of persons, such as documentation.
- 210 • State transitions – operationally significant changes between discrete states of physiological or technical conditions (for example, “modes” and “settings” for a device, “warning or alarm limit” or “action limit” for a measured physiological parameter).
- 215 • Priority may be evaluated by the original sending device or by business rules and clinical protocols in downstream systems. Sources for raw and derived data and interpretations of priority must be documented for audit/forensic purposes, potentially by additions to content of message.

X.1 Actors/Transactions

220 Figure X.1-1 shows the actors directly involved in the Infusion Pump Event Communication Integration Profile and the relevant transactions between them. Other actors that may be indirectly involved due to their participation in Device Enterprise Communications (DEC) or Point-of-care Infusion Verification (PIV), etc., are not necessarily shown.

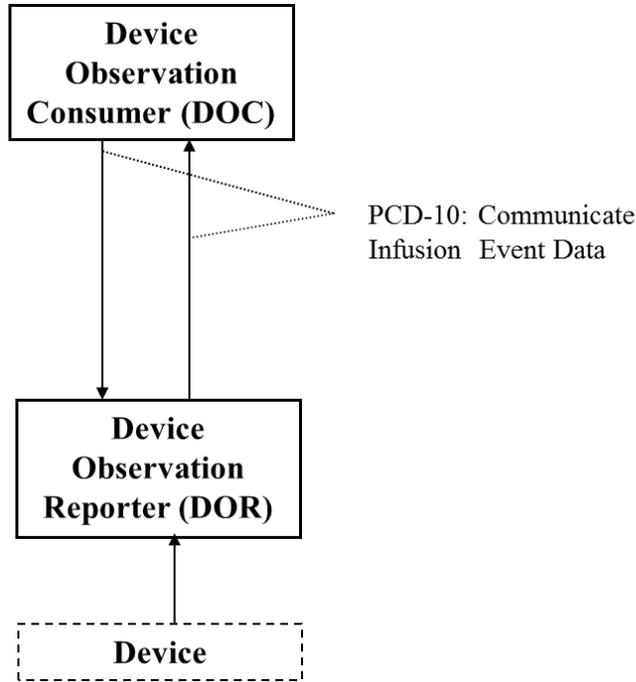

225

Figure X.1-1: Infusion Pump Event Communication Actor Diagram

230 Table X.1-1 lists the transactions for each actor directly involved in the Infusion Pump Event Communication Profile. In order to claim support of this Integration Profile, an implementation must perform the required transactions (labeled “R”). Transactions labeled “O” are optional.

Table X.1-1: Infusion Pump Event Communication Integration Profile - Actors and Transactions

Actors	Transactions	Optionality	Section in Vol. 2
Device Observation Reporter	Communicate Infusion Event Data	R	Z.1
Device Observation Consumer	Communicate Infusion Event Data	R	Z.1

235

X.2 IPEC Options

The IHE PCD Infusion Pump Event Communication profile does not define any options.

X.3 IPEC Actor Groupings and Profile Interactions

None


X.4 Infusion Pump Event Communication Process Flow

240 X.4.1 Standard Use Cases

X.4.1.1 Case IPEC-1: Communicate event data to EMR/EHR

245 Data from all of the patient care devices associated with a particular patient is communicated by a Gateway, Device or Clinical Information System (CIS) implementing the DOR actor to an EMR/EHR, implementing the DOC actor. This document only covers event data received from infusion pumps. Discrete parameters representing the device’s state at or near the time of the event are included. The data is time stamped with a consistent time across the data from the respective patient care devices.

250 The primary intent is communication of structured data; however provisions are made for inclusion of unstructured data. The application provides facilities to bind an authoritative enterprise patient identifier required for inclusion of the PCD data in the patient record. The workflow for associating the authoritative enterprise patient identifier to the PCD data is outside the scope of the current PCD TF.

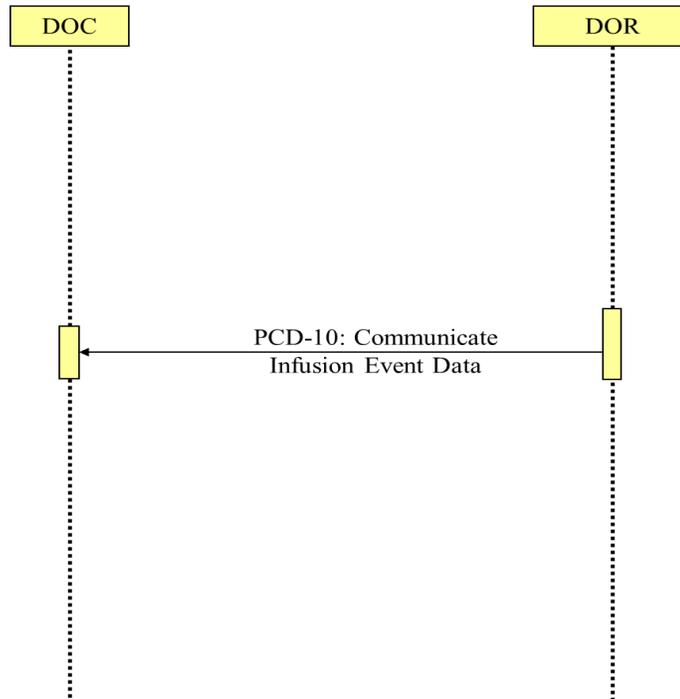

255 **Figure X.4.1.1-1: Basic Process Flow in Infusion Pump Event Communication Profile**

X.5 IPEC Security Considerations

The IPEC profile does not address issues of privacy, security, and confidentiality associated with cross-enterprise communication of PCD data. The assumption is made that the IPEC profile is implemented in a single enterprise on a secure network.

260 **Appendix A Actor Summary Definitions**

This integration profile will not add any new actors.

Appendix B Transaction Summary Definitions

265 **Infusion Pump Event** – An event, in the context of infusion pump device communications, is an occurrence about which it is desired to communicate information between Infusion Pump devices and Clinical Information Systems. For example, during normal execution of an infusion therapy, non-alarm conditions such as start of delivery, change of rate, switchover from piggyback to primary drug, completion of delivery, transition to KVO, etc., are important to full documentation of the IV administration.

270 **Glossary**

Add the following terms to the Glossary:

Event: an occurrence about which it is desired to communicate information between devices and information systems. Events include operational milestones and key parameter changes. Alarms are considered to be a subset of events.

275 **Program:** Settings used to control the operation of the pump. A program typically initiated by the clinician and entered manually on the device. Once the settings are confirmed, the clinician can then start the infusion.

280 **Auto Program:** A pump program in which some or all settings are received from another system such as an eMAR or BCMA system. When an auto-program is received on the pump, the clinician will enter any additional required settings, confirm them, and start the infusion.

Delivery: The infusion pump mechanism for moving fluid into a patient is engaged.

KVO: Keep Vein Open. A fluid delivery mode that may occur once the programmed volume has been infused.

285

Volume 2 - Transactions

Add section 3.Y

3.Y Communicate Infusion Event Data


This section corresponds to the Communicate Infusion Event Data transaction of the IHE Technical Framework. Communicate Infusion Event Data is used by the DOR and DOC actors.

290 **3.Y.1 Scope**

This transaction is used to communicate infusion event data from:

- A Device Observation Reporter (DOR) to a Device Observation Consumer (DOC).

3.Y.2 Use Case Roles

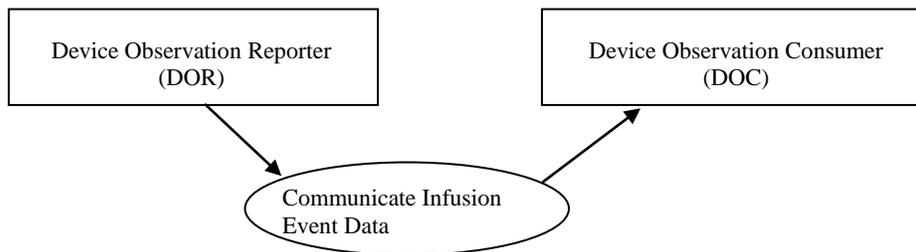

295

Actor: Device Observation Reporter

Role: Sends infusion event data to DOC

Actor: Device Observation Consumer


Role: Receives infusion event data from DOR

300

3.Y.3 Referenced Standard

- HL7 - Health Level 7 Version 2.6 Ch7 Observation Reporting
- ISO/IEEE 11073-10101 Nomenclature

305 **3.Y.4 Interaction Diagram**

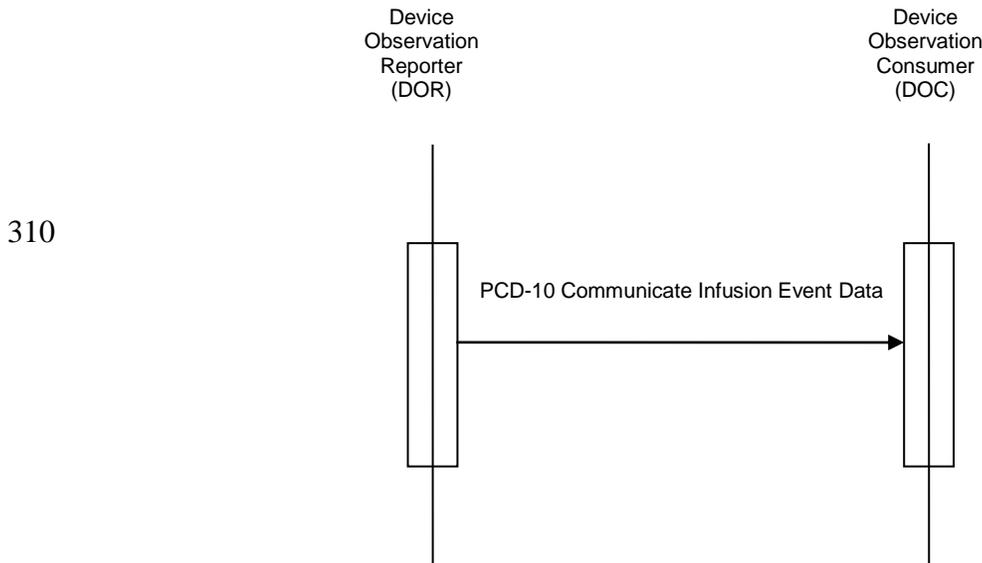

315

3.Y.4.1 Communicate Infusion Event Data

Event messages are generated by the infusion pump or Gateway during normal execution of an infusion therapy. Example of such events are start of infusion delivery, rate change or transition from piggyback to primary or transition to KVO. This information is sent from a DOR to a DOC.

320 **3.Y.4.1.1 Trigger Events**

325 The ORU^Rxx^ORU_R01 message is an unsolicited update initiated by the Device Observation Reporter. The ORU^Rxx can be sent with or without a preceding order, since it is common in a clinical setting for device data to be reported without a specific order having been transacted in the information system (that is, the reporting is the result of a "standing order" for monitoring in a particular clinical situation).

3.Y.4.1.2 Message Semantics

Refer to the HL7 standard for the ORU message of HL7 2.6 Chapter 7 and the general message semantics.

330 The ORU^Rxx^ORU_R01 message structure provides the mechanisms for mapping the hierarchical structure of an IEEE 11073 containment tree to a series of OBX messages each of which is optionally qualified by a note which immediately follows the respective OBX. See the

discussion of how the containment is represented using a "dotted notation" in field OBX-4
Observation Sub-ID in PCD Technical Framework Vol. 2 Rev. 1.2 Appendix B, Section B.8.

335 See PCD Technical Framework Vol. 2 Rev. 1.2 section 3.3 ISO/IEEE Nomenclature mapping to
HL7 OBX-3 for further information on the mapping rules.

3.Y.4.1.3 Expected Actions

The ORU^Rxx^ORU_R01 message is sent from the DOR to the DOC. Upon receipt the DOC
validates the message and responds with an acknowledgement as defined in PCD Technical
Framework Vol. 2 Rev. 1.2 Appendix G.1.1 Acknowledgment Modes.

340 Appendix X Infusion Pump Events

This appendix is intended to provide background information to support a mechanism for the
transmission of event information for large volume (general purpose) infusion pumps. Common
infusion modalities for these pumps may include continuous, piggyback, bolus, multi-step, and
intermittent functionality. Support for patient-controlled analgesia (PCA) pumps and other types
345 of pumps will be addressed at a later date.

A major challenge in reporting infusion pump events is that although pumps are able to report
programmed and operational parameters, they are typically not “aware” of how or why they are
being used clinically. In medical environments there are an enormous number of use cases for
administering an infusion using a pump. Even a routine delivery of an amount of fluid may
350 involve several instances where the infusion is paused or stopped and then restarted (either
within seconds or after several hours or more). The infusion rate may be changed, or an alarm
may cause the infusion to stop until the alarm is addressed. For various practical and clinical
reasons, the values programmed on the pump by the clinician may not relate to the volume that
the physician ordered, the actual volume of the fluid container that was hung, or the rate at which
355 the infusion was ordered.

All current pump systems do not report event information the same way. The same information
may be represented differently, or a different set of information may be reported. Information
may be reported periodically or episodically, but not in accordance with a common specification.

360 As a result, a decision has been made to standardize a small number of basic operational events.
In combination with pump mode and status information, these can be used to express the various
key operational components of an infusion over time. Systems that receive event information,
such as eMAR or BCMA systems, have the clinical/medication order information and will need
to reconcile the reported operational events with this information.

X.1 Basic Infusion Events

365 It may be helpful to think of an infusion as a series of delivery segments, each of which is
bounded by one of the following events:

- Delivery Start

- Delivery Stop
- Delivery Complete

370 There are also several other operational events not related to fluid delivery:

- Communication Status Change – communication between pump and gateway is lost or resumed
- Program Cleared – pump settings are cleared (indicating that a new program will be initiated)
- Auto-Program Cleared – an auto-program was received on the pump but the programmed settings were cleared on the pump prior to starting delivery

375

- Patient ID Change
- Patient Weight Change

The following diagram illustrates a typical scenario where a bag of fluid is infused and a rate change is made:

380

- An infusion is started at 75 mL/hr. A volume to be infused is programmed (not shown).
- After a period of time the infusion is stopped (paused), perhaps in order to move the patient.
- The infusion is resumed at 100 mL/hr.
- The programmed volume to be infused is met (delivery is complete).
- Pump switches to KVO (keep vein open) mode.

385

- Pump is stopped.

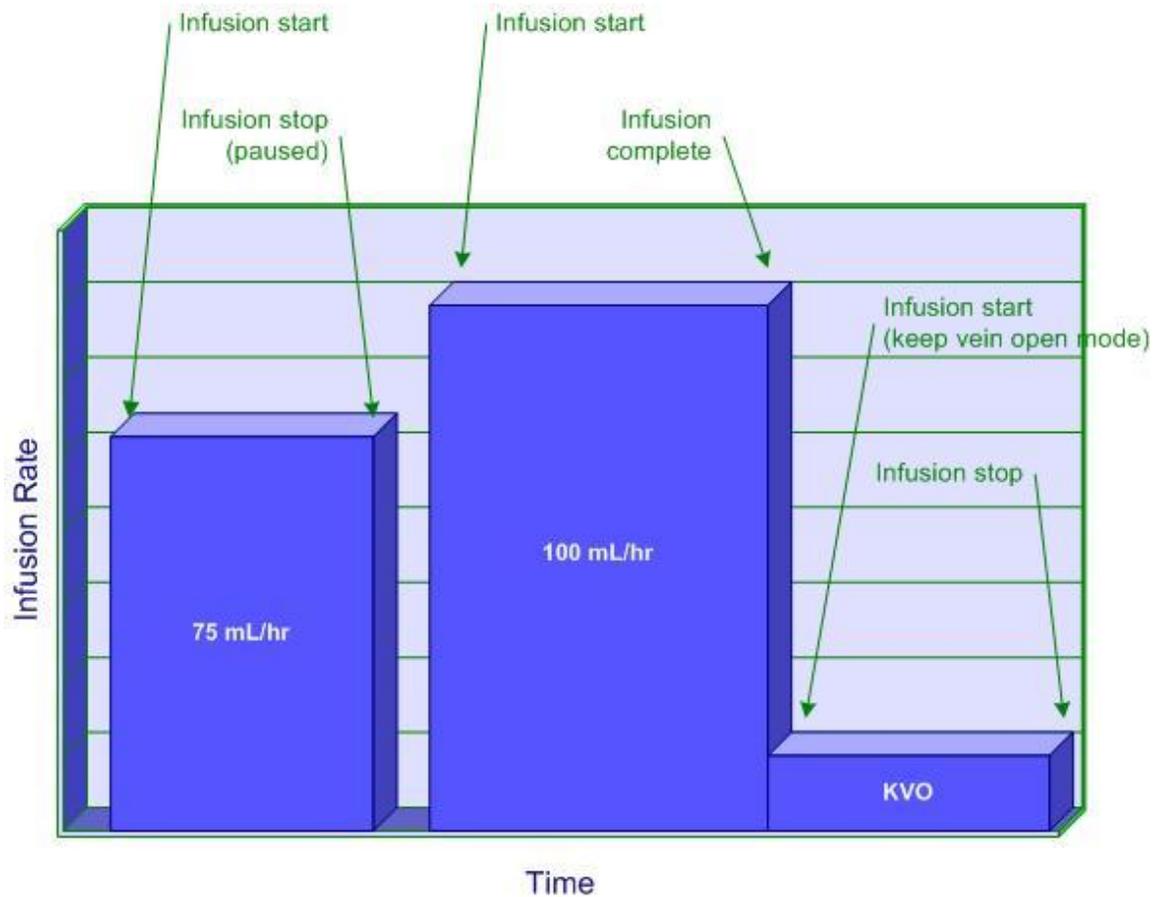


Figure X.1-1: Infusion with a Rate Change

X.1.1 Event Message – PCD-10 Communicate Infusion Event Data

390 The structure of the message differs from the PCD-01 message (ORU^R01) in the following ways

- MSH-9 contains a new trigger event code assigned for infusion event data.
- MSH-21.3 contains the PCD-10 unique profile identifier. The OID identifier assigned to PCD-10 is “1.3.6.1.4.1.19376.1.6.1.10.1”

395 Each PCD-10 message contains only information relevant to the specific device and channel on which the event occurred. Each PCD-10 message contains a single event. Only information pertinent to the event is included.

400

X.1.2 Infusion Pump Events

Table X.1.2-1: Infusion Pump Events

Event	MDC Code	Required by Profile	Containment Level
Delivery Start	MDCX_PUMP_DELIV_START	Yes	Delivery Channel*
Delivery Stop	MDCX_PUMP_DELIV_STOP	Yes	Delivery Channel*
Delivery Complete	MDCX_PUMP_DELIV_COMP	Yes	Delivery Channel*
Communication Status Change	MDCX_PUMP_COMM_STATUS_CHANGE	No	TBD
Program Cleared	MDCX_PUMP_PROG_CLEARED	No	TBD
Auto-Program Cleared	MDCX_PUMP_AUTO_PROG_CLEARED	No	TBD
Patient ID Change	MDCX_PUMP_PAT_ID_CHANGE	No	TBD
Patient Weight Change	MDCX_PUMP_PAT_WEIGHT_CHANGE	No	TBD

*Note: Delivery channel MDC expressed notation is:

405

MDC_DEV_PUMP_INFUS_VMD / MDC_DEV_PUMP_INFUS_CHAN_DELIVERY

X.1.2.1 Infusion Event Parameters

The following parameters will be used when reporting infusion events.

410

Table X.1.2.1-1: Infusion Pump Event Parameters

Parameter	MDC Code	Notes
Drug Name	MDC_DRUG_NAME_TYPE	
Drug Concentration	MDC_CONC_DRUG	
Pump Mode	MDC_PUMP_MODE	
Pump Status	MDC_PUMP_STAT	
Pump Event	MDCX_ATTR_EVT_COND	Refer to table in section 1.2.1.2 for list of events
Rate	MDC_FLOW_FLUID_PUMP	Rate (source and delivery channel)
Dose Rate	MDC_RATE_DOSE	Dose (source channel only) Used when dosing is not in mL/hr
Volume Programmed	MDC_VOL_FLUID_TBI	Volume amount to be infused (VTBI); programmed manually by

IHE Patient Care Device Technical Framework Supplement – Infusion Pump Event Communication (IPEC)

Parameter	MDC Code	Notes
		user or from PCD-03
Volume Remaining	MDC_VOL_FLUID_TBI_REMAIN	Amount of the programmed volume that is still to be infused
Volume Delivered	MDC_VOL_FLUID_DELIV	Fluid volume delivered over the last delivery segment (i.e. since the last DELIV_START) <i>Note: This amount is associated to a single channel or line (i.e., drug) – no accumulation is made across channels or lines (e.g., a bolus on top of a continuous delivery on channel A will still have its own volume delivered amounts).</i>
Cumulative Volume Delivered	MDC_VOL_FLUID_DELIV_TOTAL_SET	A counter for volume delivered that can be reset differently depending on manufacturer and model. For example, it may be reset manually by the clinician (“Clear shift totals”) or when a new patient and/or drug are selected. <i>Note: each vendor will need to outline the conditions under which this value is reset, e.g., manually, new patient, new drug, new care area) as well as how it is reported in various modes (bolus, multi-step). Because of current differences by vendor and model, this attribute is considered optional in all pump events.</i>
Time Remaining	MDC_TIME_PD_REMAIN	
Patient Height	MDC_ATTR_PT_HEIGHT	
Patient Weight	MDC_ATTR_PT_WEIGHT	
BSA (Body Surface Area)	MDC_AREA_BODY_SURF_ACTUAL	

The following tables outlines the level of containment and the required and optional attributes for each event.

Table X.1.2.1-2: Infusion Pump Delivery Events Containment and Attributes

ATTRIBUTE	CHANNEL (S)ource, (D)elivery	MDCX_PUMP_ DELIV_START	MDCX_PUMP_ DELIV_STOP	MDCX_PUMP_ DELIV_COMP
Drug Name	S	R	R	R
Concentration	S	O	O	O
Pump Mode	D	R	R	R
Pump Status	D	R	R	R

IHE Patient Care Device Technical Framework Supplement – Infusion Pump Event Communication (IPEC)

ATTRIBUTE	CHANNEL (S)ource, (D)elivery	MDCX_PUMP_ DELIV_START	MDCX_PUMP_ DELIV_STOP	MDCX_PUMP_ DELIV_COMP
Rate	D	R	R	R
	S	O	O	O
Dose Rate	S	O	O	O
Volume Programmed	S	O	O	O
Volume Remaining	S	R	R	R
Volume Delivered	S	O	R	R
Cumulative Volume Delivered	S	O	O	O
Time Remaining	S	O	O	O
Patient Height	S (or Device level)	O	O	O
Patient Weight	S (or Device level)	O	O	O
BSA (Body Surface Area)	S (or Device level)	O	O	O
<STATUS enumeration: online, offline>	N/A	N/A	N/A	N/A
<event time stamp>	N/A	N/A	N/A	N/A

415

Table X.1.2.1-3: Infusion Pump Miscellaneous Events Containment and Attributes

ATTRIBUTE	CHANNEL (S)ource, (D)elivery	MDCX_PUMP_ COMM_STATUS_ CHANGE	MDCX_PUMP_ PROG_CLEARED	MDCX_PUMP_ AUTO_PROG_ CLEARED
Drug Name	S	N/A	O	O
Concentration	S	N/A	O	O
Pump Mode	D	N/A	O	O
Pump Status	D	N/A	O	O
Rate	D	N/A	O	O
	S	N/A	O	O
Dose Rate	S	N/A	O	O
Volume Programmed	S	N/A	O	O

IHE Patient Care Device Technical Framework Supplement – Infusion Pump Event Communication (IPEC)

ATTRIBUTE	CHANNEL (S)ource, (D)elivery	MDCX_PUMP_ COMM_STATUS_ CHANGE	MDCX_PUMP_ PROG_CLEARED	MDCX_PUMP_ AUTO_PROG_ CLEARED
Volume Remaining	S	N/A	N/A	O
Volume Delivered	S	N/A	N/A	O
Cumulative Volume Delivered	S	N/A	O	O
Time Remaining	S	N/A	O	O
Patient Height	S (or Device level)	N/A	O	O
Patient Weight	S (or Device level)	N/A	O	O
BSA (Body Surface Area)	S (or Device level)	N/A	O	O
<STATUS enumeration: online, offline>	N/A	R	R	R
<event time stamp>	N/A	R	R	R

420 The following table describes the mapping of clinical scenarios to pump events. The term “delivery segment” refers to the period between a MDCX_PUMP_DELIV_START event and the next MDCX_PUMP_DELIV_STOP or MDCX_PUMP_DELIV_COMP event.

Note: Additional clinical scenarios will be added to this table as they are identified.

Table X.1.2.1-4: Clinical Scenarios

Clinical Scenario	PCD-10 Event	Required Parameters	Discussion
New infusion start, followed by eventual transition to KVO, followed by transition from KVO to paused	MDCX_PUMP_DELIV_START	<p>Mode=pump-mode-*</p> <p>Status=pump-status-infusing</p> <p>Rate(source)=programmed rate</p> <p>Rate(delivery)=programmed rate</p> <p>Dose Rate=programmed dose rate</p> <p>Volume Programmed=volume programmed</p> <p>Volume Remaining=volume programmed</p> <p>Volume Delivered=0</p> <p>Cumulative Volume Delivered=0</p> <p>Time Remaining=calculated from Volume</p>	Depending on pump make/model, Rate may not be specific to KVO rate and volume infused may continue to increase after the transition to KVO even though the VTBI has been met

IHE Patient Care Device Technical Framework Supplement – Infusion Pump Event Communication (IPEC)

Clinical Scenario	PCD-10 Event	Required Parameters	Discussion
		Remaining and Rate(source)	
	MDCX_PUMP_DELIV_COMP	<p>Mode=pump-mode-*</p> <p>Status=pump-status-vtbi-complete</p> <p>Rate(source)=programmed rate</p> <p>Rate(delivery)=0</p> <p>Dose Rate=programmed dose rate</p> <p>Volume Programmed=volume programmed</p> <p>Volume Remaining=0</p> <p>Volume Delivered= volume programmed</p> <p>Cumulative Volume Delivered= volume programmed</p> <p>Time Remaining=0</p>	
	MDCX_PUMP_DELIV_START	<p>Mode=pump-mode-continuous</p> <p>Status=pump-status-kvo</p> <p>Rate(source)=KVO rate</p> <p>Rate(delivery)=KVO rate</p> <p>Dose Rate=n/a</p> <p>Volume Programmed=0</p> <p>Volume Remaining=0</p> <p>Volume Delivered=0</p> <p>Cumulative Volume Delivered=volume programmed</p> <p>Time Remaining=0</p>	
	MDCX_PUMP_DELIV_STOP	<p>Mode=pump-mode-continuous</p> <p>Status=pump-status-paused</p> <p>Rate(source)=KVO rate</p> <p>Rate(delivery)=0</p> <p>Dose Rate=n/a</p> <p>Volume Programmed=0</p> <p>Volume Remaining=0</p> <p>Volume Delivered= volume delivered since last DELIV_START</p> <p>Cumulative Volume Delivered=volume programmed plus the amount delivered during KVO</p> <p>Time Remaining=0</p>	
Start/restart an infusion, followed by pausing the running infusion	MDCX_PUMP_DELIV_START	<p>Mode=pump-mode-*</p> <p>Status=pump-status-infusing</p> <p>Rate(source)=programmed rate</p> <p>Rate(delivery)=programmed rate</p> <p>Dose Rate=programmed dose rate</p>	

IHE Patient Care Device Technical Framework Supplement – Infusion Pump Event Communication (IPEC)

Clinical Scenario	PCD-10 Event	Required Parameters	Discussion
		<p>Volume Programmed=volume programmed Volume Remaining=volume remaining Volume Delivered=0 Cumulative Volume Delivered=sum of “Volume Delivered” values across all segments for the delivery prior to this one Time Remaining=calculated from Volume Remaining and Rate(source)</p>	
	MDCX_PUMP_DELIV_STOP	<p>Mode=pump-mode- Status=pump-status-paused Rate(source)=programmed rate Rate(delivery)=0 Dose Rate=programmed dose rate Volume Programmed=volume programmed Volume Remaining=volume remaining Volume Delivered= volume delivered since last DELIV_START Cumulative Volume Delivered=sum of “Volume Delivered” values across all segments for the delivery, including the one just completed Time Remaining=calculated from Volume Remaining and Rate(source)</p>	
Rate Change (NOTE: events associated with the start of the infusion at original rate and pausing or completion at the new rate are not shown)	MDCX_PUMP_DELIV_STOP	<p>Mode=pump-mode- Status=pump-status-paused Rate(source)=old programmed rate Rate(delivery)=0 Dose Rate=old programmed dose rate Volume Programmed=volume programmed Volume Remaining=volume remaining Volume Delivered= volume delivered since last DELIV_START Cumulative Volume Delivered=sum of “Volume Delivered” values across all segments for the delivery, including the one just completed Time Remaining=calculated from Volume Remaining and Rate(source)</p>	
	MDCX_PUMP_DELIV_START	<p>Mode=pump-mode- Status=pump-status-infusing Rate(source)=new programmed rate Rate(delivery)=new programmed rate Dose Rate=new programmed dose rate</p>	

IHE Patient Care Device Technical Framework Supplement – Infusion Pump Event Communication (IPEC)

Clinical Scenario	PCD-10 Event	Required Parameters	Discussion
		<p>Volume Programmed=volume programmed Volume Remaining=volume remaining Volume Delivered=0 Cumulative Volume Delivered=sum of “Volume Delivered” values across all segments for the delivery prior to this one Time Remaining=calculated from Volume Remaining and Rate(source)</p>	
<p>Piggyback start, followed by piggyback end, followed by resumption of the primary infusion (this assumes the pump will revert to the primary rate once piggyback VTBI is achieved)</p> <p>(NOTE: events associated with the start of the primary infusion prior to the piggyback and completion of the primary infusion after the piggyback are not shown)</p>	MDCX_PUMP_DELIV_STOP	<p>Mode=pump-mode- Status=pump-status-paused Rate(source)=primary rate Rate(delivery)=0 Dose Rate=primary dose rate Volume Programmed=primary volume programmed Volume Remaining=primary volume remaining Volume Delivered= volume delivered since last DELIV_START Cumulative Volume Delivered=sum of “Volume Delivered” values across all segments for the primary delivery, including the one just completed Time Remaining=calculated from Volume Remaining and Rate(source)</p>	<p>DELIV_STOP – Used if the pump is switching from primary to piggyback. Not needed if starting piggyback from a pause or stop.</p>
	MDCX_PUMP_DELIV_START	<p>Mode=pump-mode-piggyback Status=pump-status-infusing Rate(source)=piggyback programmed rate Rate(delivery)=piggyback programmed rate Dose Rate=piggyback dose rate Volume Programmed=piggyback volume programmed Volume Remaining=piggyback volume programmed Volume Delivered=0 Cumulative Volume Delivered=0 Time Remaining=calculated from Volume Remaining and Rate(source)</p>	
	MDCX_PUMP_DELIV_COMP	<p>Mode=pump-mode-piggyback Status=pump-status-vtbi-complete Rate(source)=piggyback programmed rate Rate(delivery)=0 Dose Rate=piggyback dose rate</p>	

IHE Patient Care Device Technical Framework Supplement – Infusion Pump Event Communication (IPEC)

Clinical Scenario	PCD-10 Event	Required Parameters	Discussion
		<p>Volume Programmed=piggyback volume programmed</p> <p>Volume Remaining=0</p> <p>Volume Delivered=volume delivered since last piggyback DELIV_START</p> <p>Cumulative Volume Delivered=sum of “Volume Delivered” values across all segments for the piggyback delivery, including the one just completed</p> <p>Time Remaining=0</p>	
	MDCX_PUMP_DELIV_START	<p>Mode=pump-mode-*</p> <p>Status=pump-status-infusing</p> <p>Rate(source)=primary rate</p> <p>Rate(delivery)=primary rate</p> <p>Dose Rate=primary dose rate</p> <p>Volume Programmed=primary volume programmed</p> <p>Volume Remaining=primary volume remaining</p> <p>Volume Delivered=0</p> <p>Cumulative Volume Delivered=sum of “Volume Delivered” values across all segments for the primary delivery</p> <p>Time Remaining=calculated from Volume Remaining and Rate(source)</p>	
<p>Bolus start, followed by bolus end, followed by resumption of continuous rate after the bolus (this assumes the pump will revert to the continuous rate once the bolus VTBI is achieved)</p> <p>(NOTE: events associated with the</p>	MDCX_PUMP_DELIV_STOP	<p>Mode=pump-mode-*</p> <p>Status=pump-status-paused</p> <p>Rate(source)=continuous rate</p> <p>Rate(delivery)=0</p> <p>Dose Rate=continuous dose rate</p> <p>Volume Programmed=continuous volume programmed</p> <p>Volume Remaining=continuous volume remaining</p> <p>Volume Delivered=continuous volume delivered since last DELIV_START</p> <p>Cumulative Volume Delivered=sum of “Volume Delivered” values across all segments for the continuous delivery, including the one just completed</p> <p>Time Remaining=calculated from Volume Remaining and Rate(source)</p>	<p>DELIV_STOP – Used if the pump is switching from continuous to bolus. Not needed if starting bolus from a pause or stop.</p>
	MDCX_PUMP_DELIV_START	<p>Mode=pump-mode-bolus</p> <p>Status=pump-status-infusing</p>	

IHE Patient Care Device Technical Framework Supplement – Infusion Pump Event Communication (IPEC)

Clinical Scenario	PCD-10 Event	Required Parameters	Discussion
<p>start of the continuous infusion prior to the bolus and completion of the continuous infusion after the bolus completes are not shown)</p>		<p>Rate(source)=bolus programmed rate Rate(delivery)=bolus programmed rate Dose Rate=bolus dose rate Volume Programmed=bolus volume programmed Volume Remaining=bolus volume programmed Volume Delivered=0 Cumulative Volume Delivered=sum of “Volume Delivered” values across all segments for the continuous delivery and any previously completed boluses Time Remaining=calculated from Volume Remaining and Rate(source)</p>	
	MDCX_PUMP_DELIV_STOP	<p>Mode=pump-mode-bolus Status=pump-status-paused Rate(source)=bolus programmed rate Rate(delivery)=0 Dose Rate=bolus dose rate Volume Programmed=bolus volume programmed Volume Remaining=0 Volume Delivered=bolus volume delivered since last DELIV_START Cumulative Volume Delivered=sum of “Volume Delivered” values across all segments for the bolus, including the one just completed, plus the sum of the “Volume Delivered” values across all segments for the continuous delivery Time Remaining=0</p>	
	MDCX_PUMP_DELIV_START	<p>Mode=pump-mode- Status=pump-status-infusing Rate(source)= continuous rate Rate(delivery)= continuous rate Dose Rate= continuous dose rate Volume Programmed= continuous volume programmed Volume Remaining= continuous volume remaining Volume Delivered=0 Cumulative Volume Delivered=sum of “Volume Delivered” values across all segments for the continuous delivery and any</p>	

IHE Patient Care Device Technical Framework Supplement – Infusion Pump Event Communication (IPEC)

Clinical Scenario	PCD-10 Event	Required Parameters	Discussion
		boluses Time Remaining=calculated from Volume Remaining and Rate(source)	
Multi-step start, followed by multi-step transition, followed by multi-step stop	MDCX_PUMP_DELIV_START	Mode=pump-mode-multi-step Status=pump-status-infusing Rate(source)=programmed rate for step 1 Rate(delivery)=programmed rate for step 1 Dose Rate=programmed dose rate for step 1 Volume Programmed=volume programmed for step 1 Volume Remaining=volume programmed for step 1 Volume Delivered=0 Cumulative Volume Delivered=0 Time Remaining=calculated from Volume Remaining and Rate(source)	The transition is handled like a rate change
	MDCX_PUMP_DELIV_STOP	Mode=pump-mode-multi-step Status=pump-status-paused Rate(source)= programmed rate for step n Rate(delivery)=0 Dose Rate= programmed dose rate for step n Volume Programmed=volume programmed for step n Volume Remaining=0 Volume Delivered= volume delivered since last DELIV_START Cumulative Volume Delivered=sum of “Volume Delivered” values across all segments for the delivery, including the one just completed Time Remaining=0	
	MDCX_PUMP_DELIV_START	Mode=pump-mode-multi-step Status=pump-status-infusing Rate(source)=programmed rate for step n+1 Rate(delivery)=programmed rate for step n+1 Dose Rate=programmed dose rate for step n+1 Volume Programmed=volume programmed for step n+1 Volume Remaining=volume programmed for step n+1 Volume Delivered=0 Cumulative Volume Delivered=sum of “Volume Delivered” values across all	

IHE Patient Care Device Technical Framework Supplement – Infusion Pump Event Communication (IPEC)

Clinical Scenario	PCD-10 Event	Required Parameters	Discussion
	MDCX_PUMP_DELIV_STOP	<p>segments for the delivery prior to this one</p> <p>Time Remaining=calculated from Volume Remaining and Rate(source)</p> <p>Mode=pump-mode-multi-step</p> <p>Status=pump-status-paused</p> <p>Rate(source)= programmed rate for current step</p> <p>Rate(delivery)=0</p> <p>Dose Rate= programmed dose rate for current step</p> <p>Volume Programmed=volume programmed for current step</p> <p>Volume Remaining=0</p> <p>Volume Delivered= volume delivered since last DELIV_START</p> <p>Cumulative Volume Delivered=sum of “Volume Delivered” values across all segments for the delivery, including the one just completed</p> <p>Time Remaining=0</p>	
Intermittent step start, followed by intermittent step stop	MDCX_PUMP_DELIV_START	<p>Mode=pump-mode-multi-dosing</p> <p>Status=pump-status-infusing</p> <p>Rate(source)=programmed rate for step n</p> <p>Rate(delivery)=programmed rate for step n</p> <p>Dose Rate=programmed dose rate for step n</p> <p>Volume Programmed=volume programmed for step n</p> <p>Volume Remaining=volume programmed for step n</p> <p>Volume Delivered=0</p> <p>Cumulative Volume Delivered=sum of “Volume Delivered” values across all segments for the delivery prior to this one</p> <p>Time Remaining=calculated from Volume Remaining and Rate(source)</p>	
	MDCX_PUMP_DELIV_STOP	<p>Mode=pump-mode-multi-dosing</p> <p>Status=pump-status-paused</p> <p>Rate(source)= programmed rate for current step</p> <p>Rate(delivery)=0</p> <p>Dose Rate= programmed dose rate for current step</p> <p>Volume Programmed=volume programmed for current step</p>	

IHE Patient Care Device Technical Framework Supplement – Infusion Pump Event Communication (IPEC)

Clinical Scenario	PCD-10 Event	Required Parameters	Discussion
		<p>Volume Remaining=0</p> <p>Volume Delivered= volume delivered since last DELIV_START</p> <p>Cumulative Volume Delivered=sum of “Volume Delivered” values across all segments for the delivery, including the one just completed</p> <p>Time Remaining=0</p>	
<p>Loading dose start, followed by loading dose end, followed by start of continuous (this assumes the pump will start at the continuous rate once the loading dose VTBI is achieved)</p> <p>(NOTE: the event associated with the completion of the continuous infusion after the bolus completes is not shown)</p>	MDCX_PUMP_DELIV_START	<p>Mode=pump-mode-loading-dose</p> <p>Status=pump-status-infusing</p> <p>Rate(source)=loading dose programmed rate</p> <p>Rate(delivery)=loading dose programmed rate</p> <p>Dose Rate=loading dose dose rate</p> <p>Volume Programmed=loading dose volume programmed</p> <p>Volume Remaining=loading dose volume programmed</p> <p>Volume Delivered=0</p> <p>Cumulative Volume Delivered=0</p> <p>Time Remaining=calculated from Volume Remaining and Rate(source)</p>	
	MDCX_PUMP_DELIV_STOP	<p>Mode=pump-mode-loading-dose</p> <p>Status=pump-status-paused</p> <p>Rate(source)=loading dose programmed rate</p> <p>Rate(delivery)=0</p> <p>Dose Rate=loading dose dose rate</p> <p>Volume Programmed=loading dose volume programmed</p> <p>Volume Remaining=0</p> <p>Volume Delivered=loading dose volume delivered since last DELIV_START</p> <p>Cumulative Volume Delivered=sum of “Volume Delivered” values across all segments for the loading dose, including the one just completed</p> <p>Time Remaining=0</p>	
	MDCX_PUMP_DELIV_START	<p>Mode=pump-mode-*</p> <p>Status=pump-status-infusing</p> <p>Rate(source)=continuous rate</p> <p>Rate(delivery)=continuous rate</p> <p>Dose Rate=continuous dose rate</p> <p>Volume Programmed=continuous volume programmed</p>	

IHE Patient Care Device Technical Framework Supplement – Infusion Pump Event Communication (IPEC)

Clinical Scenario	PCD-10 Event	Required Parameters	Discussion
		<p>Volume Remaining=continuous volume remaining</p> <p>Volume Delivered=0</p> <p>Cumulative Volume Delivered=sum of “Volume Delivered” values across all segments for the loading dose</p> <p>Time Remaining=calculated from Volume Remaining and Rate(source)</p>	
Infusion Stopped Due to Alarm			Same as “Pause a running infusion” scenario
Auto-restart after alarm resolved			e.g., occlusion resolved or AIL Same as “Start/restart an infusion” scenario
Nurse restart after alarm resolved			Same as “Start/restart an infusion” scenario
Nurse changes VTBI			e.g., bag change, hourly check, etc. Same as “Pause a running infusion” case followed by “Start/restart an infusion” case
Ramp/taper start, followed by ramp/taper rate change, followed by ramp/taper stop	MDCX_PUMP_DELIV_START	<p>Mode=pump-mode-ramp-taper</p> <p>Status=pump-status-infusing</p> <p>Rate(source)=programmed rate for step 1</p> <p>Rate(delivery)=programmed rate for step 1</p> <p>Dose Rate=programmed dose rate for step 1</p> <p>Volume Programmed=volume programmed for entire ramp/taper delivery</p> <p>Volume Remaining=volume programmed for entire ramp/taper delivery</p> <p>Volume Delivered=0</p> <p>Cumulative Volume Delivered=0</p> <p>Time Remaining=calculated from Volume Remaining and Rate(source)</p>	
	MDCX_PUMP_DELIV_STOP	<p>Mode=pump-mode-ramp-taper</p> <p>Status=pump-status-paused</p> <p>Rate(source)= programmed rate for step n</p> <p>Rate(delivery)=0</p>	

IHE Patient Care Device Technical Framework Supplement – Infusion Pump Event Communication (IPEC)

Clinical Scenario	PCD-10 Event	Required Parameters	Discussion
		<p>Dose Rate= programmed dose rate for step n</p> <p>Volume Programmed=volume programmed for entire ramp/taper delivery</p> <p>Volume Remaining=volume remaining for entire ramp/taper delivery</p> <p>Volume Delivered= volume delivered since last DELIV_START</p> <p>Cumulative Volume Delivered=sum of “Volume Delivered” values across all segments for the delivery, including the one just completed</p> <p>Time Remaining=0</p>	
	MDCX_PUMP_DELIV_START	<p>Mode=pump-mode-ramp-taper</p> <p>Status=pump-status-infusing</p> <p>Rate(source)=programmed rate for step n+1</p> <p>Rate(delivery)=programmed rate for step n+1</p> <p>Dose Rate=programmed dose rate for step n+1</p> <p>Volume Programmed=volume programmed for entire ramp/taper delivery</p> <p>Volume Remaining=volume remaining for entire ramp/taper delivery</p> <p>Volume Delivered=0</p> <p>Cumulative Volume Delivered=sum of “Volume Delivered” values across all segments for the delivery prior to this one</p> <p>Time Remaining=calculated from Volume Remaining and Rate(source)</p>	
	MDCX_PUMP_DELIV_STOP	<p>Mode=pump-mode-ramp-taper</p> <p>Status=pump-status-paused</p> <p>Rate(source)= programmed rate for step n</p> <p>Rate(delivery)=0</p> <p>Dose Rate= programmed dose rate for step n</p> <p>Volume Programmed=volume programmed for entire ramp/taper delivery</p> <p>Volume Remaining=volume remaining for entire ramp/taper delivery</p> <p>Volume Delivered= volume delivered since last DELIV_START</p> <p>Cumulative Volume Delivered=sum of “Volume Delivered” values across all segments for the delivery, including the one just completed</p> <p>Time Remaining=0</p>	
Patient ID	MDCX_PUMP_PAT_ID_CHA	New Patient ID=PID.3	

IHE Patient Care Device Technical Framework Supplement – Infusion Pump Event Communication (IPEC)

Clinical Scenario	PCD-10 Event	Required Parameters	Discussion
Change	NGE		
New Weight (same patient)	MDCX_PUMP_PAT_WEIGHT_CHANGE	Weight=New Patient Weight	e.g., when weight changed during an active weight-based infusion
Switch to library-based infusion (NOTE: events associated with the start of the non-library infusion and the completion of the library-based infusion are not shown)	MDCX_PUMP_DELIV_STOP	<p>Mode=pump-mode-*</p> <p>Status=pump-status-paused</p> <p>Rate(source)=rate of non-library infusion</p> <p>Rate(delivery)=0</p> <p>Dose Rate=dose rate of non-library infusion</p> <p>Volume Programmed=volume programmed for non-library infusion</p> <p>Volume Remaining=volume remaining of non-library infusion</p> <p>Volume Delivered= volume delivered since last DELIV_START</p> <p>Cumulative Volume Delivered=sum of “Volume Delivered” values across all segments for the non-library delivery, including the one just completed</p> <p>Time Remaining=calculated from Volume Remaining and Rate(source)</p>	The library-based infusion is considered a new delivery
	MDCX_PUMP_DELIV_START	<p>Mode=pump-mode-*</p> <p>Status=pump-status-infusing</p> <p>Rate(source)=rate of library-based infusion</p> <p>Rate(delivery)=programmed rate of library-based infusion</p> <p>Dose Rate=dose rate of library-based infusion</p> <p>Volume Programmed=volume programmed for library-based infusion</p> <p>Volume Remaining=volume programmed for library-based infusion</p> <p>Volume Delivered=0</p> <p>Cumulative Volume Delivered=0</p> <p>Time Remaining=calculated from Volume Remaining and Rate(source)</p>	
Switch from library-based infusion (NOTE: events associated with the start of the	MDCX_PUMP_DELIV_STOP	<p>Mode=pump-mode-*</p> <p>Status=pump-status-paused</p> <p>Rate(source)=rate of library infusion</p> <p>Rate(delivery)=0</p> <p>Dose Rate=dose rate of library infusion</p> <p>Volume Programmed=volume programmed for library infusion</p> <p>Volume Remaining=volume remaining of</p>	

IHE Patient Care Device Technical Framework Supplement – Infusion Pump Event Communication (IPEC)

Clinical Scenario	PCD-10 Event	Required Parameters	Discussion
library-based infusion and the completion of the non-library-based infusion are not shown)		library infusion Volume Delivered = volume delivered since last DELIV_START Cumulative Volume Delivered =sum of “Volume Delivered” values across all segments for the library delivery, including the one just completed Time Remaining =calculated from Volume Remaining and Rate(source)	
	MDCX_PUMP_DELIV_START	Mode =pump-mode- Status =pump-status-infusing Rate(source) =rate of non-library-based infusion Rate(delivery) =programmed rate of non-library-based infusion Dose Rate =dose rate of non-library-based infusion Volume Programmed =volume programmed for non-library-based infusion Volume Remaining =volume programmed for non-library-based infusion Volume Delivered =0 Cumulative Volume Delivered =0 Time Remaining =calculated from Volume Remaining and Rate(source)	

425 **X.1.2.2 Infusion Event Sample Messages**

Delivery Start Event

430 MSH|^~\&|PAT_DEVICE_PUMPVENDOR^0003B10000000001^EUI-64|PAT_DEVICE_PUMPVENDOR^0003B10000000001^EUI-64|||20100706154719-0800||ORU^Rxx^ORU_R01|PCD10_20100706154719|P|2.6||NE|AL|||EN^English^ISO659||^1.3.6.1.4.1.19376.1.6.1.10.1^ISO

PID|1||HO60002^^^PAT_DEVICE_PUMPVENDOR^MR|Darwin^Charles^^^^L||196201010000000000|M
PV1|1|I|3 West ICU^3002^1

435 OBR|1|AB12345^PCD-03|CD12345^HL7^ACDE48234567ABCD^EUI-64|2222^Dopamine
|||20100706154704-0800

OBX|1|CWE|0^MDCX_ATTR_EVT_COND^MDC|1.1.1.100|0^MDCX_PUMP_DELIV_START^MDC
||||R|||20100706154704-0800|||20100706154704-0800

OBX|2||69985^MDC_DEV_PUMP_INFUS_MDS^MDC|1.0.0.0|||||X|||||Pump002^^0003B100000000
1^EUI-64

440 OBX|3||69986^MDC_DEV_PUMP_INFUS_VMD^MDC|1.1.0.0|||||X

OBX|4||126978^MDC_DEV_PUMP_INFUS_CHAN_DELIVERY^MDC|1.1.1.0|||||X

OBX|5|ST|184508^MDC_PUMP_STAT^MDC|1.1.1.101|^pump-status-
infusing||||R|||20100706154704-0800|||20100706154704-0800

445 OBX|6|ST|184504^MDC_PUMP_MODE^MDC|1.1.1.102|^pump-mode-
continuous||||R|||20100706154704-0800|||20100706154704-0800

OBX|7|NM|157784^MDC_FLOW_FLUID_PUMP^MDC|1.1.1.103|24.9|265266^MDC_DIM_MILLI_L_PER_HR^M
DC^mL/h^mL/h^UCUM||||R|||20100706154704-0800|||20100706154704-0800

OBX|8||126977^MDC_DEV_PUMP_INFUS_CHAN_SOURCE^MDC|1.1.2.0|||||X

450 OBX|9|ST|184330^MDC_DRUG_NAME_TYPE^MDC|1.1.2.201|Dopamine||||R|||20100706154704-
0800|||20100706154704-0800

OBX|10|NM|157760^MDC_CONC_DRUG^MDC|1.1.2.202|1.6|264306^MDC_DIM_MILLI_G_PER_ML^MDC^mg/
mL^mg/mL^UCUM||||R|||20100706154704-0800|||20100706154704-0800

OBX|11|NM|157924^MDC_RATE_DOSE^MDC|1.1.2.203|7|265619^MDC_DIM_MICRO_G_PER_KG_PER_MIN^M
DC^ug/kg/min^ug/kg/min^UCUM||||R|||20100706154704-0800|||20100706154704-0800

455 OBX|12|NM|157784^MDC_FLOW_FLUID_PUMP^MDC|1.1.2.204|24.9|265266^MDC_DIM_MILLI_L_PER_HR^
MDC^mL/h^mL/h^UCUM||||R|||20100706154704-0800|||20100706154704-0800

OBX|13|NM|999999^MDC_VOL_FLUID_TBI^MDC|1.1.2.205|250|263762^MDC_DIM_MILLI_L^MDC^mL^mL^
UCUM||||R|||20100706154704-0800|||20100706154704-0800

460 OBX|14|NM|157872^MDC_VOL_FLUID_TBI_REMAIN^MDC|1.1.2.206|250|263762^MDC_DIM_MILLI_L^MDC
^mL^mL^UCUM||||R|||20100706154704-0800|||20100706154704-0800

OBX|15|NM|157864^MDC_VOL_FLUID_DELIV^MDC|1.1.2.207|0|263762^MDC_DIM_MILLI_L^MDC^mL^mL^
UCUM||||R|||20100706154704-0800|||20100706154704-0800

OBX|16|NM|157888^MDC_VOL_FLUID_DELIV_TOTAL_SET^MDC|1.1.2.208|0|263762^MDC_DIM_MILLI_L^
MDC^mL^mL^UCUM||||R|||20100706154704-0800|||20100706154704-0800

465 OBX|17|NM|68063^MDC_ATTR_PT_WEIGHT^MDC|1.1.2.209|95|263875^MDC_DIM_KILO_G^MDC^kg^kg^UC
UM||||R|||20100706154704-0800|||20100706154704-0800

Delivery Stop Event

- 470 MSH|^~\&|PAT_DEVICE_PUMPVENDOR^0003B1000000001^EUI-64|PAT_DEVICE_PUMPVENDOR^0003B1000000001^EUI-64|||20100706163708-0800||ORU^Rxx^ORU_R01|PCD10_20100706163708|P|2.6||NE|AL|||EN^English^ISO659|||^1.3.6.1.4.1.19376.1.6.1.10.1^ISO
PID|1||HO60002^^^PAT_DEVICE_PUMPVENDOR^MR||Darwin^Charles^^^^L||196201010000000000|M
PV1|1|I|3 West ICU^3002^1
- 475 OBR|1|AB12345^PCD-03|CD12345^HL7^ACDE48234567ABCD^EUI-64|2222^Dopamine
|||20100706163629-0800
OBX|1|CWE|0^MDCX_ATTR_EVT_COND^MDC|1.1.1.100|
0^MDCX_PUMP_DELIV_STOP^MDC|||||R|||20100706163629-0800|||20100706163629-0800
OBX|2||69985^MDC_DEV_PUMP_INFUS_MDS^MDC|1.0.0.0|||||X|||||Pump002^^0003B1000000000
1^EUI-64
- 480 OBX|3||69986^MDC_DEV_PUMP_INFUS_VMD^MDC|1.1.0.0|||||X
OBX|4||126978^MDC_DEV_PUMP_INFUS_CHAN_DELIVERY^MDC|1.1.1.0|||||X
OBX|5|ST|184508^MDC_PUMP_STAT^MDC|1.1.1.101|^pump-status-
paused|||||R|||20100706163629-0800|||20100706163629-0800
- 485 OBX|6|ST|184504^MDC_PUMP_MODE^MDC|1.1.1.102|^pump-mode-
continuous|||||R|||20100706163629-0800|||20100706163629-0800
OBX|7|NM|157784^MDC_FLOW_FLUID_PUMP^MDC|1.1.1.103|0|265266^MDC_DIM_MILLI_L_PER_HR^MDC^
mL/h^mL/h^UCUM|||||R|||20100706163629-0800|||20100706163629-0800
OBX|8||126977^MDC_DEV_PUMP_INFUS_CHAN_SOURCE^MDC|1.1.2.0|||||X
- 490 OBX|9|ST|184330^MDC_DRUG_NAME_TYPE^MDC|1.1.2.201|Dopamine|||||R|||20100706163629-
0800|||20100706163629-0800
OBX|10|NM|157760^MDC_CONC_DRUG^MDC|1.1.2.202|1.6|264306^MDC_DIM_MILLI_G_PER_ML^MDC^mg/
mL^mg/mL^UCUM|||||R|||20100706163629-0800|||20100706163629-0800
OBX|11|NM|157924^MDC_RATE_DOSE^MDC|1.1.2.203|7|265619^MDC_DIM_MICRO_G_PER_KG_PER_MIN^M
DC^ug/kg/min^ug/kg/min^UCUM|||||R|||20100706163629-0800|||20100706163629-0800
- 495 OBX|12|NM|157784^MDC_FLOW_FLUID_PUMP^MDC|1.1.2.204|24.9|265266^MDC_DIM_MILLI_L_PER_HR^
MDC^mL/h^mL/h^UCUM|||||R|||20100706163629-0800|||20100706163629-0800
OBX|13|NM|999999^MDC_VOL_FLUID_TBI^MDC|1.1.2.205|250|263762^MDC_DIM_MILLI_L^MDC^mL^mL^
UCUM|||||R|||20100706163629-0800|||20100706163629-0800
- 500 OBX|14|NM|157872^MDC_VOL_FLUID_TBI_REMAIN^MDC|1.1.2.206|224.4|263762^MDC_DIM_MILLI_L^M
DC^mL^mL^UCUM|||||R|||20100706163629-0800|||20100706163629-0800
OBX|15|NM|157864^MDC_VOL_FLUID_DELIV^MDC|1.1.2.207|25.6|263762^MDC_DIM_MILLI_L^MDC^mL^
mL^UCUM|||||R|||20100706163629-0800|||20100706163629-0800
OBX|16|NM|999999^MDC_VOL_FLUID_DELIV_TOTAL_SET^MDC|1.1.2.208|25.6|263762^MDC_DIM_MILLI
_L^MDC^mL^mL^UCUM|||||R|||20100706163629-0800|||20100706163629-0800
- 505 OBX|17|NM|68063^MDC_ATTR_PT_WEIGHT^MDC|1.1.2.209|95|263875^MDC_DIM_KILO_G^MDC^kg^kg^UC
UM|||||R|||20100706163629-0800|||20100706163629-0800

Delivery Complete Event

- 510 MSH|^~\&|PAT_DEVICE_PUMPVENDOR^0003B1000000001^EUI-64|PAT_DEVICE_PUMPVENDOR^0003B1000000001^EUI-64|||20100707023629-0800||ORU^Rxx^ORU_R01|PCD10_20100706163708|P|2.6||NE|AL|||EN^English^ISO659|||^1.3.6.1.4.1.19376.1.6.1.10.1^ISO
PID|1||HO60002^^^PAT_DEVICE_PUMPVENDOR^MR||Darwin^Charles^^^L||196201010000000000|M
- 515 PV1|1|I|3 West ICU^3002^1
OBR|1|AB12345^PCD-03|CD12345^HL7^ACDE48234567ABCD^EUI-64|2222^Dopamine|||20100707023629-0800
OBX|1|CWE|0^MDCX_ATTR_EVT_COND^MDC|1.1.1.100|0^MDCX_PUMP_DELIV_COMP^MDC|||||R|||20100707023629-0800|||||20100707023629-0800
- 520 OBX|2||69985^MDC_DEV_PUMP_INFUS_MDS^MDC|1.0.0.0|||||X|||||Pump002^^0003B1000000001^EUI-64
OBX|3||69986^MDC_DEV_PUMP_INFUS_VMD^MDC|1.1.0.0|||||X
OBX|4||126978^MDC_DEV_PUMP_INFUS_CHAN_DELIVERY^MDC|1.1.1.0|||||X
OBX|5|ST|184508^MDC_PUMP_STAT^MDC|1.1.1.101|^pump-status-vtbi-complete|||||R|||20100707023629-0800|||||20100707023629-0800
OBX|6|ST|184504^MDC_PUMP_MODE^MDC|1.1.1.102|^pump-mode-continuous|||||R|||20100707023629-0800|||||20100707023629-0800
OBX|7|NM|157784^MDC_FLOW_FLUID_PUMP^MDC|1.1.1.103|0|265266^MDC_DIM_MILLI_L_PER_HR^MDC^mL/h^mL/h^UCUM|||||R|||20100707023629-0800|||||20100707023629-0800
- 530 OBX|8||126977^MDC_DEV_PUMP_INFUS_CHAN_SOURCE^MDC|1.1.2.0|||||X
OBX|9|ST|184330^MDC_DRUG_NAME_TYPE^MDC|1.1.2.201|Dopamine|||||R|||20100707023629-0800|||||20100707023629-0800
OBX|10|NM|157760^MDC_CONC_DRUG^MDC|1.1.2.202|1.6|264306^MDC_DIM_MILLI_G_PER_ML^MDC^mg/mL^mg/mL^UCUM|||||R|||20100707023629-0800|||||20100707023629-0800
- 535 OBX|11|NM|157924^MDC_RATE_DOSE^MDC|1.1.2.203|7|265619^MDC_DIM_MICRO_G_PER_KG_PER_MIN^MDC^ug/kg/min^ug/kg/min^UCUM|||||R|||20100707023629-0800|||||20100707023629-0800
OBX|12|NM|157784^MDC_FLOW_FLUID_PUMP^MDC|1.1.2.204|24.9|265266^MDC_DIM_MILLI_L_PER_HR^MDC^mL/h^mL/h^UCUM|||||R|||20100707023629-0800|||||20100707023629-0800
- 540 OBX|13|NM|999999^MDC_VOL_FLUID_TBI^MDC|1.1.2.205|250|263762^MDC_DIM_MILLI_L^MDC^mL^mL^UCUM|||||R|||20100707023629-0800|||||20100707023629-0800
OBX|14|NM|157872^MDC_VOL_FLUID_TBI_REMAIN^MDC|1.1.2.206|0.0|263762^MDC_DIM_MILLI_L^MDC^mL^mL^UCUM|||||R|||20100707023629-0800|||||20100707023629-0800
OBX|15|NM|157864^MDC_VOL_FLUID_DELIV^MDC|1.1.2.207|224.4|263762^MDC_DIM_MILLI_L^MDC^mL^mL^UCUM|||||R|||20100707023629-0800|||||20100707023629-0800
- 545 OBX|16|NM|999999^MDC_VOL_FLUID_DELIV_TOTAL_SET^MDC|1.1.2.208|250.0|263762^MDC_DIM_MILLI_L^MDC^mL^mL^UCUM|||||R|||20100707023629-0800|||||20100707023629-0800
OBX|17|NM|68063^MDC_ATTR_PT_WEIGHT^MDC|1.1.2.209|95|263875^MDC_DIM_KILO_G^MDC^kg^kg^UCUM|||||R|||20100707023629-0800|||||20100707023629-0800