

Integrating the Healthcare Enterprise



5

**IHE Radiology  
Technical Framework Supplement**

10

**Web-based Image Capture  
(WIC)**

15

**Rev. 1.4 – Trial Implementation**

20      Date:        August 6, 2020  
Author:        IHE Radiology Technical Committee  
Email:         [radiology@ihe.net](mailto:radiology@ihe.net)

25

**Please verify you have the most recent version of this document.** See [here](#) for Trial Implementation and Final Text versions and [here](#) for Public Comment versions.

## Foreword

This is a supplement to the IHE Radiology Technical Framework V19.0. Each supplement undergoes a process of public comment and trial implementation before being incorporated into the volumes of the Technical Frameworks.

This supplement is published on August 6, 2020 for trial implementation and may be available for testing at subsequent IHE Connectathons. The supplement may be amended based on the results of testing. Following successful testing it will be incorporated into the Radiology Technical Framework. Comments are invited and may be submitted at [http://www.ihe.net/Radiology\\_Public\\_Comments](http://www.ihe.net/Radiology_Public_Comments).

This supplement describes changes to the existing technical framework documents.

“Boxed” instructions like the sample below indicate to the Volume Editor how to integrate the relevant section(s) into the relevant Technical Framework volume.

*Amend Section X.X by the following:*

Where the amendment adds text, make the added text **bold underline**. Where the amendment removes text, make the removed text **bold strikethrough**. When entire new sections are added, introduce with editor’s instructions to “add new text” or similar, which for readability are not bolded or underlined.

General information about IHE can be found at [www.ihe.net](http://www.ihe.net).

Information about the IHE Radiology domain can be found at [ihe.net/IHE Domains](http://ihe.net/IHE_Domains).

Information about the organization of IHE Technical Frameworks and Supplements and the process used to create them can be found at [http://ihe.net/IHE Process](http://ihe.net/IHE_Process) and <http://ihe.net/Profiles>.

The current version of the IHE Radiology Technical Framework can be found at [http://www.ihe.net/Technical\\_Frameworks](http://www.ihe.net/Technical_Frameworks).

55

## CONTENTS

	Introduction to this Supplement.....	5
60	Open Issues and Questions .....	5
	Closed Issues.....	5
	IHE Technical Frameworks General Introduction.....	7
65	9 Copyright Licenses.....	7
	9.1 Copyright of Base Standards .....	7
	9.1.1 DICOM (Digital Imaging and Communications in Medicine).....	7
	9.1.2 HL7 (Health Level Seven).....	7
	9.1.3 LOINC (Logical Observation Identifiers Names and Codes) .....	7
	9.1.4 SNOMED CT (Systematized Nomenclature of Medicine -- Clinical Terms).....	8
	10 Trademark .....	8
70	IHE Technical Frameworks General Introduction Appendices.....	9
	Appendix A – Actor Summary Definitions .....	9
	Appendix B – Transaction Summary Definitions.....	9
	Appendix D – Glossary.....	9
	<b>Volume 1 – Profiles .....</b>	<b>10</b>
75	38 Web-based Image Capture (WIC) Profile.....	10
	38.1 WIC Actors, Transactions, and Content Modules .....	10
	38.1.1 Actor Descriptions and Actor Profile Requirements .....	11
	38.1.1.1 Image Manager.....	11
	38.2 WIC Actor Options .....	11
	38.2.1 JPEG Storage Option .....	12
80	38.2.2 MPEG4 Storage Option .....	12
	38.2.3 Evidence Document Storage Option .....	12
	38.2.4 DICOM Instance Storage Option.....	12
	38.2.5 PNG Storage Option.....	12
	38.2.6 QuickTime Storage Option .....	12
85	38.2.7 3GPP Storage Option .....	12
	38.3 WIC Required Actor Groupings .....	13
	38.4 WIC Overview .....	13
	38.4.1 Concepts .....	13
	38.4.2 Use Cases .....	13
90	38.4.2.1 Use Case #1: Image Upload to a New Study .....	13
	38.4.2.1.1 Image Upload to a New Study Use Case Description .....	13
	38.4.2.2 Use Case #2: Image Upload to an Existing Study.....	14
	38.4.2.2.1 Image Upload to an Existing Study Use Case Description .....	14
	38.4.2.2.2 Image Upload to an Existing Study Process Flow.....	14
95	38.5 WIC Security Considerations.....	15
	38.6 WIC Cross Profile Considerations .....	16
	<b>Volume 2 – Transactions .....</b>	<b>17</b>
	4.108 Store Instances over the Web [RAD-108] .....	17

---

	4.108.1 Scope .....	17
100	4.108.2 Actor Roles.....	17
	4.108.3 Referenced Standards.....	17
	4.108.4 Messages .....	18
	4.108.4.1 Store Instances Message.....	18
	4.108.4.1.1 Trigger Events .....	18
105	4.108.4.1.2 Message Semantics .....	18
	4.108.4.1.2.1 Capture Device Attribute Requirements.....	19
	4.108.4.1.2.2 Lightweight Modality Attribute Requirements.....	20
	4.108.4.1.2.3 Single-frame Image.....	20
	4.108.4.1.2.3.1 JPEG Storage Option .....	21
110	4.108.4.1.2.3.2 PNG Storage Option .....	21
	4.108.4.1.2.4 Multi-frame Video .....	21
	4.108.4.1.2.4.1 MPEG4 Storage Option .....	22
	4.108.4.1.2.4.2 QuickTime Storage Option .....	22
	4.108.4.1.2.4.3 3GPP Storage Option .....	22
115	4.108.4.1.2.5 Evidence Document Storage Option.....	23
	4.108.4.1.2.6 DICOM Instance Storage Option.....	24
	4.108.4.1.3 Expected Actions .....	24
	4.108.4.1.3.1 PNG Storage Option .....	25
	4.108.4.1.3.2 QuickTime Storage Option .....	25
120	4.108.4.1.3.3 3GPP Storage Option.....	26
	4.108.4.2 Return Status Message .....	26
	4.108.4.2.1 Trigger Events .....	26
	4.108.4.2.2 Message Semantics .....	26
	4.108.4.2.3 Expected Actions .....	26
125	4.108.5 Security Considerations.....	26
	4.108.5.1 Security Audit Considerations.....	26
	4.108.5.2 Transport Security .....	26
	<b>Volume 3 – Cross-Transaction Specifications.....</b>	<b>27</b>
130		

## Introduction to this Supplement

There is an increasing use of mobile devices such as smartphones or tablets for image capture or viewing in healthcare. For example, a clinician can use a tablet to launch an image viewer via the EMR. The camera on the mobile device can capture high quality still images and videos.

- 135 However, there is no standard way for these devices to upload captured images or evidence documents directly to the Image Manager.

The Web-based Image Capture (WIC) Profile provides a simple, lightweight, mobile-friendly mechanism to encode and send captured images, videos and evidence documents from the mobile device to the Image Manager so that these objects can be easily integrated into the rest of the imaging workflow.

140

The Encounter-based Imaging Workflow (EBIW) Profile complements WIC and provides a more comprehensive solution to handle image acquisition on smartphones, cameras, etc. Readers of WIC are highly encouraged to also read EBIW.

## Open Issues and Questions

145

No open issues.

## Closed Issues

1	Should the Receiver be required to convert QuickTime (.mov) into MPEG-4 (.mp4)? iOS can only create QuickTime video encoded as H.264 video stream. QuickTime is not a DICOM supported video container format.  Ans: Closed. Named option in Image Manager.
2	Should the Receiver be required to convert .3GP into MPEG-4? Other devices (e.g., Blackberry) use .3GP container for its MPEG-4 encoded video stream. It is used in older version of mobile SDKs, but newer version supports MP4 container directly.  Ans: Closed. Named option in Image Manager.
3	Should the Receiver be required to convert PNG into lossless JPEG (.70) Most mobile SDK supports creation of images using JPEG (lossy) or PNG (lossless). JPEG is compatible with DICOM while PNG is not.  Ans: Closed. Named option in Image Manager.
4	Should a Receiver be added that doesn't have to convert to binary instances? Ans: No. The Receiver must support returning binary instances upon request.

5	<p>Should each media type be a separate transaction?</p> <p>Currently there is only one transaction and each media type is a named option.</p> <p>Ans: Keep one transaction.</p>
6	<p>Do we need to add H.265 video?</p> <p>Newer mobile SDK (e.g., iOS 8) supports creating video encoded in H.265 which is not yet supported by DICOM.</p> <p>Ans: Closed. Do not support H.265 encoding now. Feedback is still welcome.</p>
7	<p>Are specific details needed for the AVC / H.264 video bit stream to be compatible with the DICOM Transfer Syntax?</p> <p>Ans: Closed. WIC does not specify any more specific details other than the use of AVC/H.264. Feedback is still welcome.</p>
8	<p>Should there be more specific details about the PNG encoding?</p> <p>Ans: Closed. Added 8-bit per channel.</p>
9	<p>Should WIC also support audio or waveform capture?</p> <p>Ans: Closed. No suitable SOP Class in DICOM for general audio capture. If business case exists, then perhaps a new encapsulated audio IOD can be introduced. Feedback is still welcome.</p>
10	<p>Should the different contents be named options or defer to product documents?</p> <p>Ans: Closed. Named option.</p>
11	<p>For evidence document with bulk data, should the media type of the payload be generic application/octet-stream or more specific application/pdf for PDF and text/xml for CDA?</p> <p>Currently STOW-RS expects using the generic octet-stream.</p> <p>Ans: Specific for PDF and CDA. Submit CP to DICOM WG-27.</p>
12	<p>Should support for encapsulated PDF and CDA be in scope or not?</p> <p>Ans: In scope.</p>
13	<p>What should the Receiver use in the response message body (JSON or XML)?</p> <p>Currently STOW-RS allows either XML or JSON in the response message body.</p> <p>The Receiver should honor the HTTP Accept field.</p> <p>What if it accepts both? Match what was used in the Request?</p> <p>Ask WG-27 about 6.6.1.3. Intention is to stay compatible with STOW-RS</p> <p>Ans: Closed. Add note in Expected Action on Receiver to honor HTTP Accept field.</p>

## IHE Technical Frameworks General Introduction

150 The [IHE Technical Framework General Introduction](#) is shared by all of the IHE domain technical frameworks. Each technical framework volume contains links to this document where appropriate.

## 9 Copyright Licenses

- 155 IHE International hereby grants to each Member Organization, and to any other user of these documents, an irrevocable, worldwide, perpetual, royalty-free, nontransferable, nonexclusive, non-sublicensable license under its copyrights in any IHE profiles and Technical Framework documents, as well as any additional copyrighted materials that will be owned by IHE International and will be made available for use by Member Organizations, to reproduce and distribute (in any and all print, electronic or other means of reproduction, storage or transmission) such IHE Technical Documents.
- 160 The licenses covered by this Copyright License are only to those copyrights owned or controlled by IHE International itself. If parts of the Technical Framework are included in products that also include materials owned or controlled by other parties, licenses to use those products are beyond the scope of this IHE document and would have to be obtained from that other party.

### 9.1 Copyright of Base Standards

165 IHE technical documents refer to and make use of a number of standards developed and published by several standards development organizations. All rights for their respective base standards are reserved by these organizations. This agreement does not supersede any copyright provisions applicable to such base standards. Copyright license information for frequently referenced base standards is provided below.

#### 9.1.1 DICOM (Digital Imaging and Communications in Medicine)

DICOM® is the registered trademark of the National Electrical Manufacturers Association for its standards publications relating to digital communications of medical information.

#### 9.1.2 HL7 (Health Level Seven)

175 HL7®, Health Level Seven®, CDA®, and FHIR® are registered trademarks of Health Level Seven International.

Health Level Seven, Inc. has granted permission to IHE to reproduce tables from the HL7 standard. The HL7 tables in this document are copyrighted by Health Level Seven, Inc. All rights reserved. Material drawn from these documents is credited where used.

#### 9.1.3 LOINC (Logical Observation Identifiers Names and Codes)

180 LOINC® is registered United States trademarks of Regenstrief Institute, Inc.

#### **9.1.4 SNOMED CT (Systematized Nomenclature of Medicine -- Clinical Terms)**

185 Some IHE Profiles incorporate SNOMED® CT, which is used by permission of the International Health Terminology Standards Development Organisation. SNOMED CT® was originally created by the College of American Pathologists. SNOMED CT is a registered trademark of the International Health Terminology Standards Development Organisation, all rights reserved.

### **10 Trademark**

190 IHE® and the IHE logo are trademarks of the Healthcare Information Management Systems Society in the United States and trademarks of IHE Europe in the European Community. They may only be used with the written consent of the IHE International Board Operations Committee, which may be given to a Member Organization in broad terms for any use that is consistent with the IHE mission and operating principles.

## IHE Technical Frameworks General Introduction Appendices

195 The [IHE Technical Framework General Introduction Appendices](#) are components shared by all of the IHE domain technical frameworks. Each technical framework volume contains links to these documents where appropriate.

### Appendix A – Actor Summary Definitions

*Add the following new or modified actors to the IHE Technical Frameworks General Introduction Appendix A:*

200

New (or modified) Actor Name	Definition
Image Capturer	A creator of DICOM composite instances.

The table below lists *existing* actors that are utilized in this profile.

#### Complete List of Existing Actors Utilized in this Profile

Existing Actor Name	Definition
Image Manager	Stores DICOM objects without guarantee of long-term storage.

205

### Appendix B – Transaction Summary Definitions

*Add the following new or modified transactions to the IHE Technical Frameworks General Introduction Appendix B:*

New (or modified) Transaction Name and Number	Definition
Store Instances over the Web [RAD-108]	Store one or more DICOM instances using DICOMweb STOW-RS.

210

### Appendix D – Glossary

*Add the following new or updated glossary terms to the IHE Technical Frameworks General Introduction Appendix D.*

None

215

# Volume 1 – Profiles

## 220 38 Web-based Image Capture (WIC) Profile

There is an increasing use of mobile devices such as smartphones or tablets for image capture or viewing in healthcare. For example, a clinician can use a tablet to launch an image viewer via the EMR. The camera on the mobile device can capture high quality still images and videos.


225 However, there is no standard way for these devices to upload captured images or evidence documents directly to the Image Manager.

The Web-based Image Capture (WIC) Profile provides a simple, lightweight, mobile-friendly mechanism to encode and send captured images, videos and evidence documents from the mobile device to the Image Manager so that these objects can be easily integrated into the rest of the imaging workflow.

## 230 38.1 WIC Actors, Transactions, and Content Modules

This section defines the actors, transactions, and/or content modules in this profile. General definitions of actors are given in the Technical Frameworks General Introduction Appendix A at [http://ihe.net/Technical\\_Frameworks](http://ihe.net/Technical_Frameworks).

235 Figure 38.1-1 shows the actors directly involved in the WIC Profile and the relevant transactions between them. If needed for context, other actors that may be indirectly involved due to their participation in other related profiles are shown in dotted lines. Actors which have a mandatory grouping are shown in conjoined boxes.

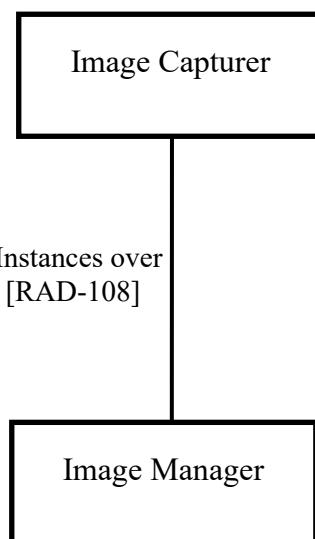

240

**Figure 38.1-1: WIC Actor Diagram**

Table 38.1-1 lists the transactions for each actor directly involved in the WIC Profile. To claim compliance with this profile, an actor shall support all required transactions (labeled “R”) and may support the optional transactions (labeled “O”).

**Table 38.1-1: WIC Profile - Actors and Transactions**

<b>Actors</b>	<b>Transactions</b>	<b>Optionality</b>	<b>TF Reference</b>
Image Capturer	Store Instances over the Web [RAD-108]	R	RAD TF-2: 4.108.1
Image Manager	Store Instances over the Web [RAD-108]	R	RAD TF-2: 4.108.1

245

### 38.1.1 Actor Descriptions and Actor Profile Requirements

Most requirements are documented in Transactions (Volume 2 and 3). This section documents any additional requirements on this profile’s actors.

#### 38.1.1.1 Image Manager

- 250 The Image Manager is required to support JPEG, MPEG4, DICOM Instance and Evidence Document Storage.

### 38.2 WIC Actor Options

Options that may be selected for each actor in this profile, if any, are listed in the Table 38.2-1. Dependencies between options when applicable are specified in notes.

255

**Table 38.2-1: WIC - Actors and Options**

<b>Actor</b>	<b>Option Name</b>	<b>TF Reference</b>
Image Capturer	JPEG Storage (Note 1)	Section 38.2.1
	MPEG4 Storage (Note 1)	Section 38.2.2
	Evidence Document Storage (Note 1)	Section 38.2.3
	DICOM Instance Storage (Note 1)	Section 38.2.4
	PNG Storage (Note 1)	Section 38.2.5
	QuickTime Storage (Note 1)	Section 38.2.6
	3GPP Storage (Note 1)	Section 38.2.7
Image Manager (Note 2)	PNG Storage	Section 38.2.5
	QuickTime Storage	Section 38.2.6
	3GPP Storage	Section 38.2.7

Note 1: The Image Capturer shall support at least one option.

Note 2: The Image Manager is required to support JPEG, MPEG4, DICOM Instance and Evidence Document Storage.

### **38.2.1 JPEG Storage Option**

- 260 The Image Capturer captures still images in baseline JPEG format (i.e., DICOM Transfer Syntax 1.2.840.10008.1.2.4.50) and stores to the Image Manager using the DICOM PS3.18 metadata and bulk data. See RAD TF-2: 4.108.4.1.2.3.1.

### **38.2.2 MPEG4 Storage Option**

- 265 The Image Capturer captures video stream encoded in AVC/H.264 format using a MP4 container and stores to the Image Manager using the DICOM PS3.18 metadata and bulk data. See RAD TF-2: 4.108.4.1.2.4.1.

### **38.2.3 Evidence Document Storage Option**

- 270 The Image Capturer supports creation of DICOM instances using DICOM Native XML Format or JSON Metadata format for evidence documents such as GSPS, SR, KOS, and DICOM Encapsulated PDF/CDA. See RAD TF-2: 4.108.4.1.2.5.

### **38.2.4 DICOM Instance Storage Option**

The Image Capturer supports creation or transmissions of DICOM instances encoded in DICOM binary format. See RAD TF-2: 4.108.4.1.2.6.

### **38.2.5 PNG Storage Option**

- 275 The Image Capturer supports creation of images in lossless PNG format. See RAD TF-2: 4.108.4.1.2.3.2.

The Image Manager supports storing images in lossless PNG format and conversion of PNG images to an appropriate standard uncompressed or lossless (reversible) compressed Transfer Syntax. See RAD TF-2: 4.108.4.1.3.1.

280 **38.2.6 QuickTime Storage Option**

The Image Capturer supports creation of video encoded in AVC/H.264 using the QuickTime container. See RAD TF-2: 4.108.4.1.2.4.2.

- 285 The Image Manager supports storing videos in AVC/H.264 video stream contained in a QuickTime (.mov) container and conversion of the video stream from a QuickTime container to a MP4 container. See also RAD TF-2: 4.108.4.1.3.2.

### **38.2.7 3GPP Storage Option**

The Image Capturer supports creation of video encoded in AVC/H.264 using the 3GPP container. See RAD TF-2: 4.108.4.1.2.4.3.

- 290 The Image Manager supports storing videos in AVC/H.264 video stream contained in a 3GPP (.3gp) container and conversion of the video stream from a 3GPP container to a MP4 container. See RAD TF-2: 4.108.4.1.3.3.

### 38.3 WIC Required Actor Groupings

295 An actor from this profile (Column 1) shall implement all of the required transactions and/or content modules in this profile ***in addition to*** all of the transactions required for the grouped actor (Column 2).

Section 38.5 describes some optional groupings that may be of interest for security considerations and Section 38.6 describes some optional groupings in other related profiles.

**Table 38.3-1: WIC - Required Actor Groupings**

WIC Actor	Actor to be grouped with	Reference
Image Capturer	None	--
Image Manager	None	--

300 **38.4 WIC Overview**

#### 38.4.1 Concepts

The Web-based Image Capture Profile enables an imaging-enabled client application running on a wide variety of devices (ranging from workstation to lightweight mobile devices) to transmit DICOM instances to the server using HTTP(S).

305 Instead of creating a DICOM PS3.10 binary instance, WIC supports DICOM PS3.18 which defines the Native DICOM Model in XML and a DICOM JSON Object Model. This enables non-traditional imaging clients (such as the clients might be used in wound care department, dermatology, etc.) to create proper DICOM instances using common tools like XML and JSON.

#### 38.4.2 Use Cases

310 **38.4.2.1 Use Case #1: Image Upload to a New Study**

##### 38.4.2.1 Image Upload to a New Study Use Case Description


Clinical Use Case: A nurse in the wound care department sees patients in the ward. She photographs the wounds to track the healing process. She uses one of the department's photo cameras, a departmental tablet or her mobile phone to take a series of pictures of a patient. She immediately imports the images in the imaging system under the correct patient name and adds an appropriate report note in the patient chart.

This use case is addressed by the Lightweight Modality in the Encounter-Based Imaging Workflow (EBIW) Profile. EBIW incorporates the Store Instances over the Web [RAD-108] transaction defined by WIC for RESTful storage of images.

320 **38.4.2.2 Use Case #2: Image Upload to an Existing Study****38.4.2.2.1 Image Upload to an Existing Study Use Case Description**

**Clinical Use Case:** A radiologist uses a tablet to retrieve a study from the central repository. While viewing the study, she identifies certain key images and adds some markup indicating the region of interest. Finally, she creates a report. When she saves the changes, the application sends the markups, key objects and reports to the central repository for persistent storage.


325 **Technical Use Case 1:** The Imaging Document Consumer retrieves and views a study from the Imaging Document Source using the Web-based Image Access (WIA) Profile. The Imaging Document Consumer, grouped with the Image Capturer, creates new evidence documents (e.g., Key Image Notes, screen captures as Secondary Capture, etc.) using the same patient and study context. The Image Capturer then uploads the created evidence documents to the Image Manager.

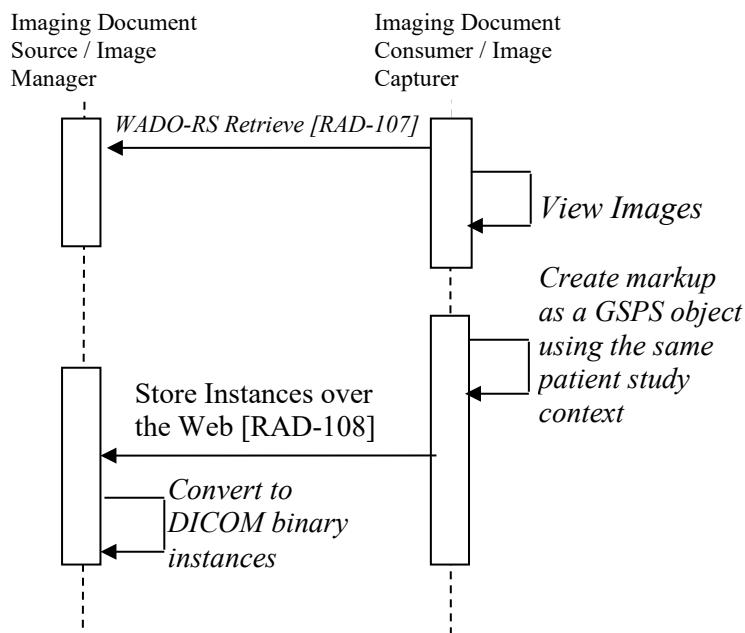**38.4.2.2.2 Image Upload to an Existing Study Process Flow**

**Figure 38.4.2.2.2-1: Image Upload to an Existing Study Process Flow in WIC Profile**

335 **Technical Use Case 2:** Similarly, using the Invoke Image Display (IID) Profile, an EMR, as an Image Display Invoker, launches an Image Display to view a patient's study. Using the markup tools and key image tools provided by the Image Display, the user creates new markups and tag certain images as key images. The IID Image Display, grouped with the Image Capturer, stores the markup and key images in the same patient and study context to the Image Manager using DICOM JSON Object Model. The Image Manager receives the instances and converts them into

DICOM binary format. Another Image Display (not part of this profile), which is a traditional PACS workstation, retrieves the study and presents the markup as well as key images.

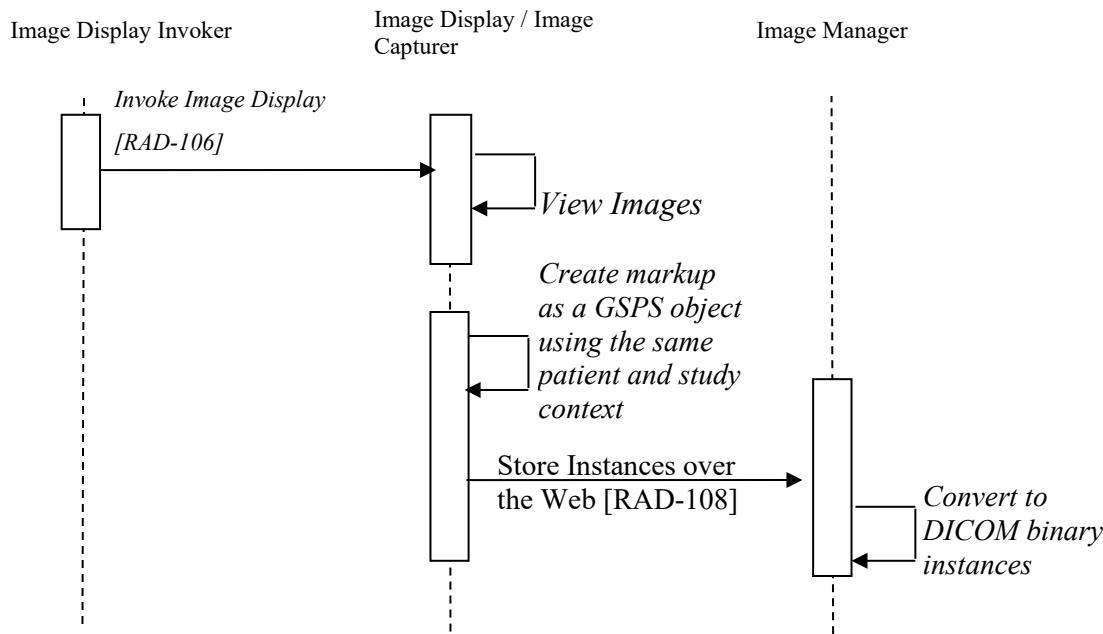

**Figure 38.4.2.2.2-2: Image Upload to an Existing Study Process Flow in WIC Profile**

## 345    38.5 WIC Security Considerations

Since the Image Capturer may be running in a mobile device outside of the hospital private network, it is important to ensure that the communication between the Image Capturer and the Image Manager is secure. Encryption specified in the ITI Audit Trail and Node Authentication (ATNA) Profile can provide secure data transport. ATNA audit messages can ensure audit trails for private health information are captured.

350 It is recommended that the Image Manager will be grouped with the ATNA Secure Node or Secure Application to record audit messages for the transactions performed. It is not expected that the Image Capturer will record audit messages.

355 The Image Manager may want to restrict which users are authorized to upload. The ITI Internet User Authorization (IUA) Profile provides OAuth-based user authorization.

The Image Manager may want to restrict which devices are authorized to upload. ATNA provides certificate-based node authentication.

360 Since the Image Capturer may be running in a mobile device that can easily be lost, it is important to consider how much information should be retained in the mobile device. This includes patient demographics as well as the images, videos or reports.

## 38.6 WIC Cross Profile Considerations

### IID – Invoke Image Display

An Image Capturer might be grouped with an Image Display in the Invoke Image Display Profile to create and store evidence documents back to the associated Image Manager based on images being viewed and their associated patient and study context.

365

### XDS-I.b – Cross-Enterprise Document Sharing for Imaging

An Image Capturer might be grouped with an XDS-I.b Imaging Document Consumer to create and store new objects back to the Image Manager based on study objects it is viewing.

370

An Image Manager might be grouped with an XDS-I.b Imaging Document Source to receive objects sent from an Image Capturer and publish a new manifest.

### WIA – Web-based Image Access

An Image Capturer might be grouped with an WIA Imaging Document Consumer to create and store new objects back to the Image Manager based on study objects it is viewing.

375

An Image Manager might be grouped with an WIA Imaging Document Source to receive objects sent from an Image Capturer.

### PDQm – Patient Demographics Query for Mobile

An Image Capturer might be grouped with a PDQm Patient Demographics Consumer to retrieve reliable patient demographics from the Patient Demographics Supplier.

# Volume 2 – Transactions

380

*Add Section 4.108*

## 4.108 Store Instances over the Web [RAD-108]

### 4.108.1 Scope

This transaction is used by the Sender to send well-formed DICOM composite objects in either DICOM binary format, or in metadata and bulk data format to the Receiver for storage.

385

The instances may be images, video, DICOM evidence documents (such as Key Image Notes, or Presentation States) or binary DICOM objects. Typically, the instances will have been newly created by the Sender. The instances may be sent as part of an existing DICOM Study, or part of a new Study.

### 4.108.2 Actor Roles

390

The Roles in this transaction are defined in the following table and may be played by the actors shown here:

**Table 4.108.2-1: Actor Roles**

<b>Role:</b>	<b>Sender:</b> Creates and sends well-formed DICOM composite objects
<b>Actor(s):</b>	The following actors may play the role of Sender:  Image Capturer Lightweight Modality
<b>Role:</b>	<b>Receiver:</b> Receives objects from the Sender
<b>Actor(s):</b>	The following actors may play the role of Receiver:  Image Manager

395

Transaction text specifies behavior for each Role. The behavior of specific actors may also be specified when it goes beyond that of the general Role.

### 4.108.3 Referenced Standards

DICOM PS3.3: Information Object Definitions

DICOM PS3.4: Service Class Specifications

DICOM PS3.5 Section B.2: UUID Derived UID

400

([http://medical.nema.org/medical/dicom/current/output/chtml/part05/sect\\_B.2.html](http://medical.nema.org/medical/dicom/current/output/chtml/part05/sect_B.2.html))

DICOM PS3.18 Section 10.5: Store Transaction (STOW-RS)


([http://medical.nema.org/medical/dicom/current/output/html/part18.html#sect\\_10.5](http://medical.nema.org/medical/dicom/current/output/html/part18.html#sect_10.5))

DICOM PS3.19 Section A.1: Native DICOM Model

ISO/IEC 14496-14:2003: MPEG-4 Part 14

405

## 4.108.4 Messages

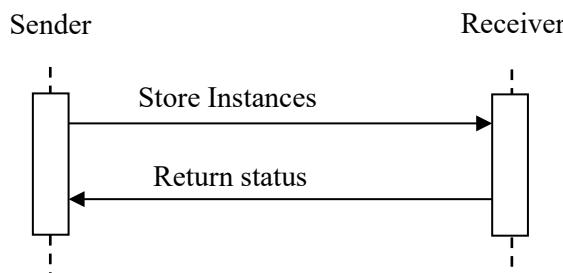

**Figure 4.108.4-1: Interaction Diagram**

### 4.108.4.1 Store Instances Message

The Sender creates one or more instances and sends these instances to the Receiver for storage.

410

There may be one or more Senders storing instances to the same Receiver at any given time.

#### 4.108.4.1.1 Trigger Events

User or application initiates transfer of the acquired or created instances to the Receiver.

#### 4.108.4.1.2 Message Semantics

This message is a DICOM STOW-RS request. The Sender is the User-Agent. The Receiver is the Origin-Server.

415

The Sender shall use the Store Instances action type.

The Sender shall encode the instances using either the binary DICOM method or the DICOM PS3.18 metadata and bulk data method.

The Sender shall encode the metadata and bulk data request in one of the following two manners:

420

- Array of DICOM JSON Model Object as defined in DICOM PS3.18 Annex F
- XML request messages as defined in the Native DICOM Model defined in DICOM PS3.19 with one message part per XML object

Note: STOW-RS specifies Native DICOM Model as a baseline and JSON Model Object is optional. In WIC, the Sender may support either one.

425

If the Sender needs to create new unique identifiers (e.g., for Study Instance UID, Series Instance UID or SOP Instance UID), it shall do so using UUID Derived UID mechanism specified in DICOM PS3.5 Section B.2.

Details about when it is appropriate to trigger the creation of a new Study/Series/SOP Instance are described in RAD TF-2: 4.8.4.1.1.1 “Study UIDs and Series UIDs”.

#### 430 4.108.4.1.2.1 Capture Device Attribute Requirements

A Sender that is a Capture Device shall populate patient demographics according to Table 4.108.4.1.2-1 in order to provide the appropriate patient context for the created DICOM Instances. Additional patient demographics can be populated by the Sender according to DICOM PS3.3 C.7.1.1.

- 435 Note: The means by which the Sender obtains the existing study values to populate these attributes is not specified here but might include using another transaction, extracting them from the integrated viewer, or via the user interface provided by the Sender.

**Table 4.108.4.1.2-1: Critical Patient Demographics Attributes**

DICOM Attribute	Opt.	Existing Study Case (RAD TF-1: 38.4.2.2)
Patient's Name (0010,0010)	R	Equal to existing study
Patient ID (0010,0020)	R	Equal to existing study
Issuer of Patient ID (0010,0021)	R	Equal to existing study
Patient's Birth Date (0010,0030)	R	Equal to existing study
Patient's Sex (0010,0040)	R	Equal to existing study

- 440 When sending metadata, the Sender shall populate Type 1 study attributes and also Type 2 study attributes for which the value is known. If a reliable source of metadata attributes is available, values from that source shall be used; otherwise the Sender shall populate study attributes according to Table 4.108.4.1.2-2. The Sender populates additional study attributes according to DICOM PS3.3 C.7.2.1 and C.7.3.1. The study attributes may be populated by either extracting  
445 the study attributes from the integrated viewer, or via the user interface provided by the Sender.

**Table 4.108.4.1.2-2: Critical Study Attributes**

DICOM Attribute	Opt.	Existing Study Case (RAD TF-1: 38.4.2.2)
Study Instance UID (0020,000D)	R	Equal to existing study
Accession Number (0008,0050)	R	Equal to existing study
Issuer of Accession Number Sequence (0008,0051)	R	Equal to existing study
Series Date (0008,0021)	R	Acquisition date
Series Time (0008,0031)	R	Acquisition time
Series Description (0008,103E)	R	Possibly pre-configured or user input
Performed Procedure Step ID (0040,0253)	O	Internally generated
Performed Procedure Step Start Date (0040,0244)	O	Acquisition date
Performed Procedure Step Start Time (0040,0245)	O	Acquisition time

DICOM Attribute	Opt.	Existing Study Case (RAD TF-1: 38.4.2.2)
Performed Procedure Step Description (0040,0254)	O	Possibly pre-configured, user input, or from existing study
Request Attribute Sequence (0040,0275)		
> Reason for Requested Procedure (0040,1002)	R	Possibly pre-configured, user input, or from existing study
> Reason for Requested Procedure Code Sequence (0040,100A)	O	Possibly pre-configured, user input, or from existing study

#### 4.108.4.1.2.2 Lightweight Modality Attribute Requirements

450 A Sender that is a Lightweight Modality in the Encounter-Based Imaging Workflow (EBIW) Profile shall populate metadata attributes as shown in Table 4.131.4.1.2-1.

#### 4.108.4.1.2.3 Single-frame Image

The Sender shall encode compressed single-frame image pixel data elements in one message part per instance.

455 The Sender shall include all required attributes in the Native DICOM Model or DICOM JSON Model Object according to DICOM PS3.4 Section B.5 for the appropriate DICOM SOP Class.

Table 4.108.4.1.2.3-1 identifies recommended SOP Classes for commonly captured single-frame image types. DICOM defines more specific SOP Classes that may be used if applicable (see DICOM PS3.3).

**Table 4.108.4.1.2.3-1: Recommended SOP Classes for Single-frame Images**

Captured Image Type	SOP Class Name	SOP Class UID	IOD Specification defined in DICOM PS3.3
Photographs	VL Photographic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.4	VL Photographic Image IOD
Screenshots	Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	Secondary Capture Image IOD

460 The Image Pixel Module is mandatory according to DICOM PS3.3 except when using STOW-RS when its attributes may be omitted according to DICOM PS3.18 Section 10.5.1.4. This exception is due to the limitation to obtain the image pixel information by certain mobile SDK or mobile clients (e.g., zero footprint browser client

**Table 4.108.4.1.2.3-2: Image Pixel Macros Attributes**

Attribute Name	Tag
Samples per Pixel	(0028,0002)
Photometric Interpretation	(0028,0004)
Rows	(0028,0010)

Attribute Name	Tag
Columns	(0028,0011)
Bits Allocated	(0028,0100)
Bits Stored	(0028,0101)
High Bit	(0028,0102)
Pixel Representation	(0028,0103)

465

#### 4.108.4.1.2.3.1 JPEG Storage Option

A Sender that supports the JPEG Storage Option shall be capable of sending images that are created using JPEG compression.

470 If the Sender knows the Transfer Syntax of the JPEG image, the Sender shall encode the compressed pixel data using single-frame Media Types described in DICOM PS3.18 Table 8.7.3-5.

If the Sender does not know the Transfer Syntax of the JPEG image, the Sender shall use a media type of image/jpeg.

#### 4.108.4.1.2.3.2 PNG Storage Option

475 A Sender that claims the PNG Storage Option shall be capable of creating images using lossless PNG compression with 8-bit per channel.

The Sender shall use a media type of image/png.

#### 4.108.4.1.2.4 Multi-frame Video

480 The Sender shall encode compressed multi-frame video pixel data elements in one message part per instance.

The Sender shall include all required attributes in the Native DICOM Model or DICOM JSON Model Object according to DICOM PS3.4 Section B.5 for the appropriate DICOM SOP Class.

485 Table 4.108.4.1.2.4-1 identifies recommended SOP Classes for commonly captured multi-frame video types. DICOM defines more specific SOP Classes that may be used if applicable (see DICOM PS3.3).

**Table 4.108.4.1.2.4-1: Recommended SOP Classes for Multi-frame Videos**

Captured Video Type	SOP Class Name	SOP Class UID	IOD Specification defined in DICOM PS3.3
Video Photographs	Video Photographic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.4.1	Video Photographic Image IOD

- 490 The Image Pixel Module is mandatory according to DICOM PS3.3 except when using STOW-RS when its attributes may be omitted according to DICOM PS3.18 Section 10.5.1.4. This exception is due to the limitation to obtain the image pixel information by certain mobile SDK or mobile clients (e.g., zero footprint browser client).

**Table 4.108.4.1.2.4-2: Image Pixel Macro Attributes**

Element Name	Tag
Samples per Pixel	(0028,0002)
Photometric Interpretation	(0028,0004)
Rows	(0028,0010)
Columns	(0028,0011)
Bits Allocated	(0028,0100)
Bits Stored	(0028,0101)
High Bit	(0028,0102)
Pixel Representation	(0028,0103)

#### 4.108.4.1.2.4.1 MPEG4 Storage Option

- 495 A Sender that supports the MPEG4 Storage Option shall be capable of sending videos that are encoded using AVC/H.264.

If the Sender knows the Transfer Syntax of the created video, the Sender shall encode the compressed video stream using a Media Type described in DICOM PS3.18 Table 8.7.3-5.

- 500 If the Sender does not know the Transfer Syntax of the created video and the created video is using an MPEG4 container, then the Sender shall use the video/mp4 media type.

The Sender shall support at least the video/mp4 media type. When using the video/mp4 media type, the MPEG-4 video stream shall be encoded using the AVC/H.264 encoding scheme and stored in the MP4 container format (ISO/IEC 14496-14:2003).

#### 4.108.4.1.2.4.2 QuickTime Storage Option

- 505 A Sender that supports the QuickTime Storage Option shall be capable of creating video stream encoded using the AVC/H.264 encoding scheme and stored in the QuickTime container format.

The Sender shall use a media type of video/quicktime.

#### 4.108.4.1.2.4.3 3GPP Storage Option

- 510 A Sender that supports the 3GPP Storage Option shall be capable of creating video stream encoded using the AVC/H.264 encoding scheme and stored in the 3GPP container format.

The Sender shall use a media type of video/3gpp.

#### 4.108.4.1.2.5 Evidence Document Storage Option

The Sender shall encode the complete evidence document metadata in the first part of the multipart request.

- 515 The Sender shall include all required attributes in the Native DICOM Model or DICOM JSON Model Object according to DICOM PS3.4 Section B.5 for the appropriate DICOM SOP Class that is used for the evidence document.

- 520 Table 4.108.4.1.2.5-1 identifies recommended SOP Classes for commonly created evidence documents. DICOM defines more specific SOP Classes that may be used if applicable (see DICOM PS3.3).

**Table 4.108.4.1.2.5-1: Recommended SOP Classes for Evidence Document**

Captured Evidence Document Type	SOP Class Name	SOP Class UID	IOD Specification defined in DICOM PS3.3
Presentation State	Grayscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.1	Grayscale Softcopy Presentation State IOD
	Color Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.2	Color Softcopy Presentation State IOD
	Pseudo-Color Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.3	Pseudo-color Softcopy Presentation State IOD
Structured Report	Basic Text SR	1.2.840.10008.5.1.4.1.1.88.11	Basic Text SR IOD
	Enhanced SR	1.2.840.10008.5.1.4.1.1.88.22	Enhanced SR IOD
	Comprehensive SR	1.2.840.10008.5.1.4.1.1.88.33	Comprehensive SR IOD
	Comprehensive 3D SR	1.2.840.10008.5.1.4.1.1.88.34	Comprehensive 3D SR IOD
Key Object Selection	Key Object Selection Document	1.2.840.10008.5.1.4.1.1.88.59	Key Object Selection Document IOD
Encapsulated Document	Encapsulated PDF Storage	1.2.840.10008.5.1.4.1.1.104.1	Encapsulated PDF IOD
	Encapsulated CDA Storage	1.2.840.10008.5.1.4.1.1.104.2	Encapsulated CDA IOD

The Sender shall include each encapsulated document in its own separate message part in the DICOM Request Message Body with the following HTTP headers:

- 525
- Encapsulated PDF document
    - Content-Type: application/pdf
    - Content-Location: {BulkDataURI}
  - Encapsulated CDA document
    - Content-Type: text/xml

- 530
  - Content-Location: {BulkDataURI}
  - Other encapsulated document
    - Content-Type: application/octet-stream
    - Content-Location: {BulkDataURI}

The expected endpoint for DICOM Encapsulated PDF / CDA documents is a DICOM server.

- 535      For transmission of plain PDF or CDA documents that are not intended to be DICOM encapsulated and stored to a DICOM server, the ITI Mobile Access to Health Document (MHD) Profile provides a more appropriate mechanism for uploading electronic health records.

#### **4.108.4.1.2.6 DICOM Instance Storage Option**

The Image Capturer shall encode each DICOM instance as a separate message part.

- 540      The Image Capturer shall send the DICOM instances using DICOM binary format.

#### **4.108.4.1.3 Expected Actions**

The Receiver shall accept and process the message payload.

- 545      The Receiver shall accept metadata and bulk data encoded in either Native DICOM Model or DICOM JSON Model Object. The Receiver shall at least support the SOP Classes defined in Tables 4.108.4.1.2.3-1, 4.108.4.1.2.4-1 and 4.108.4.1.2.5-1.

If the message contents are not binary DICOM instances, the Receiver shall convert the DICOM metadata and bulk data into DICOM binary instances according to the SOP Class UID specified in the metadata.

- 550      If the received object includes empty Image Pixel Macro Attributes (see Table 4.108.4.1.2-1), the Receiver shall populate them according to the Image Pixel Attribute Descriptions specified in DICOM PS3.3 Section C.7.6.3.1.

The Receiver shall store the DICOM binary instances (either received or converted) such that they can be later queried or retrieved in a fashion meeting the requirements defined for a DICOM Level 2 Storage SCP (refer to DICOM PS3.4 Section B.4.1).

- 555      If the received object includes the Transfer Syntax in the media type parameter, then the Receiver shall use the same Transfer Syntax when converting the DICOM metadata and bulk data into DICOM binary instances.

- 560      If the media type of the received object is image/jpeg, then the Receiver shall use the Transfer Syntax 1.2.840.10008.1.2.4.50 when converting the DICOM metadata and bulk data into DICOM binary instances.

If the media type of the received object is video/mpeg or video/mp4, then the Receiver shall use the appropriate Transfer Syntax for the received object as defined in the following table:

**Table 4.108.4.1.3-1: Transfer Syntaxes for Video**

<b>Media Type</b>	<b>Eligible Transfer Syntax</b>	<b>Description</b>
video/mpeg	1.2.840.10008.1.2.4.100	MPEG2 Main Profile @ Main Level
	1.2.840.10008.1.2.4.101	MPEG2 Main Profile @ High Level
video/mp4	1.2.840.10008.1.2.4.102	MPEG-4 AVC/H.264 High Profile / Level 4.1
	1.2.840.10008.1.2.4.103	MPEG-4 AVC/H.264 BD-compatible High Profile / Level 4.1
	1.2.840.10008.1.2.4.104	MPEG-4 AVC/H.264 High Profile / Level 4.2 for 2D Video
	1.2.840.10008.1.2.4.105	MPEG-4 AVC/H.264 High Profile / Level 4.2 for 3D Video
	1.2.840.10008.1.2.4.106	MPEG-4 AVC/H.264 Stereo High Profile / Level 4.2

## 565    **4.108.4.1.3.1 PNG Storage Option**

A Receiver that supports the PNG Storage Option shall convert the encoded lossless PNG image into DICOM binary format with an appropriate standard uncompressed or lossless (reversible) compressed Transfer Syntax.

**Table 4.108.4.1.3.1-1: Eligible Transfer Syntaxes for PNG Storage**

<b>Media Type</b>	<b>Eligible Transfer Syntax</b>	<b>Description</b>
image/png	1.2.840.10008.1.2	Implicit VR Little Endian: Default Transfer Syntax for DICOM
	1.2.840.10008.1.2.1	Explicit VR Little Endian
	1.2.840.10008.1.2.1.99	Deflated Explicit VR Little Endian
	1.2.840.10008.1.2.4.57	JPEG Lossless, Non-Hierarchical (Process 14)
	1.2.840.10008.1.2.4.70	JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 [Selection Value 1]): Default Transfer Syntax for Lossless JPEG Image Compression
	1.2.840.10008.1.2.4.80	JPEG-LS Lossless Image Compression
	1.2.840.10008.1.2.4.90	JPEG 2000 Image Compression (Lossless Only)
	1.2.840.10008.1.2.4.92	JPEG 2000 Part 2 Multi-component Image Compression (Lossless Only)
	1.2.840.10008.1.2.5	RLE Lossless

570

## **4.108.4.1.3.2 QuickTime Storage Option**

A Receiver that supports this QuickTime Storage Option shall convert the encoded QuickTime video into DICOM binary format with the pixel data encoding using appropriate Transfer Syntax defined in Table 4.108.4.1.3-1.

575 **4.108.4.1.3.3 3GPP Storage Option**

A Receiver that supports this 3GPP Storage Option shall convert the encoded 3GPP video into DICOM binary format with the pixel data encoding using appropriate Transfer Syntax defined in Table 4.108.4.1.3-1.

**4.108.4.2 Return Status Message**

- 580 The Receiver reports the outcome of the Store Instances Message.

**4.108.4.2.1 Trigger Events**

The Receiver receives a Store Instances Message.

**4.108.4.2.2 Message Semantics**

- 585 This message is a DICOM STOW-RS response. The Sender is the User-Agent. The Receiver is the Origin-Server.

The Receiver shall return a response to the Sender according to DICOM PS3.18 Section 10.5.3.

Note: The Receiver may return a response before all processing is complete for the received object; for example, performing required image conversion asynchronously after sending the response. Sender implementers should be aware that such post-response processing may fail.

- 590 Note: The Receiver will honor the HTTP Accept header field for encoding of the response message. However, if the Sender accepts both XML and JSON, then the Receiver can choose either format for the response message.

**4.108.4.2.3 Expected Actions**

The Sender has no expected actions.

**4.108.5 Security Considerations**

595 **4.108.5.1 Security Audit Considerations**

The Radiology Audit Trail Option in the IHE ITI Audit Trail and Node Authentication Profile (ITI TF-1:9) defines audit requirements for IHE Radiology transactions. See RAD TF-3: 5.1.1.

**4.108.5.2 Transport Security**

- 600 In order to avoid unauthorized interception of private health information, the communication over HTTP may be secured by using HTTPS.

# Volume 3 – Cross-Transaction Specifications

605

*Update Volume 3, Table 5.1-2 to add a new row for RAD-108. Note that transactions are listed in numeric order.*

**Table 5.1-2: IHE Radiology transactions and resulting ATNA trigger events**

IHE Radiology Transaction	ATNA Trigger Event(s)	Actor(s) that shall be able to record audit event
Patient Registration [RAD-1]	Patient-record-event	ADT Order Placer, DSS/OF - when PHI is presented
...		
<b><u>Store Instances over the Web [RAD-108]</u></b>	<b><u>Instances-stored</u></b>	<b><u>Receiver: Image Manager</u></b>
...		

610