

**Integrating the Healthcare Enterprise**



5

**IHE Radiology  
Technical Framework Supplement**

10

**Web-based Image Capture  
(WIC)**

15

**Rev. 1.5 – Trial Implementation**

20 Date: March 10, 2022  
Author: IHE Radiology Technical Committee  
Email: radiology@ihe.net

25

**Please verify you have the most recent version of this document. See [here](#) for Trial Implementation and Final Text versions and [here](#) for Public Comment versions.**

## Foreword

30 This is a supplement to the IHE Radiology Technical Framework V20.0. Each supplement undergoes a process of public comment and trial implementation before being incorporated into the volumes of the Technical Frameworks.

This supplement is published on March 10, 2022 for trial implementation and may be available for testing at subsequent IHE Connectathons. The supplement may be amended based on the results of testing. Following successful testing it will be incorporated into the Radiology  
35 Technical Framework. Comments are invited and may be submitted at [Radiology Public Comments](#).

This supplement describes changes to the existing technical framework documents.

“Boxed” instructions like the sample below indicate to the Volume Editor how to integrate the relevant section(s) into the relevant Technical Framework volume.

40 

<i>Amend Section X.X by the following:</i>
--

Where the amendment adds text, make the added text **bold underline**. Where the amendment removes text, make the removed text **~~bold strikethrough~~**. When entire new sections are added, introduce with editor’s instructions to “add new text” or similar, which for readability are not bolded or underlined.

45

General information about IHE can be found at [IHE.net](#).

Information about the IHE Radiology domain can be found at [IHE Domains](#).

Information about the organization of IHE Technical Frameworks and Supplements and the process used to create them can be found at [Profiles](#) and [IHE Process](#).

50 The current version of the IHE Radiology Technical Framework can be found at [Radiology Technical Framework](#).

55 **CONTENTS**

	Introduction to this Supplement.....	5
	Open Issues and Questions .....	5
	Closed Issues.....	5
60	IHE Technical Frameworks General Introduction.....	7
	9 Copyright Licenses.....	7
	10 Trademark .....	7
	IHE Technical Frameworks General Introduction Appendices.....	8
	Appendix A – Actors .....	8
65	Appendix B – Transactions.....	8
	Appendix D – Glossary.....	9
	<b>Volume 1 – Profiles .....</b>	<b>10</b>
	38 Web-based Image Capture (WIC) Profile.....	10
	38.1 WIC Actors, Transactions, and Content Modules .....	10
70	38.1.1 Actor Descriptions and Actor Profile Requirements .....	11
	38.1.1.1 Image Manager.....	11
	38.2 WIC Actor Options .....	11
	38.2.1 JPEG Storage Option .....	11
	38.2.2 MPEG4 Storage Option .....	12
75	38.2.3 Evidence Document Storage Option .....	12
	38.2.4 DICOM Instance Storage Option.....	12
	38.2.5 PNG Storage Option.....	12
	38.3 WIC Required Actor Groupings .....	12
	38.4 WIC Overview .....	12
80	38.4.1 Concepts .....	12
	38.4.2 Use Cases .....	13
	38.4.2.1 Use Case #1: Image Upload to a New Study .....	13
	38.4.2.1.1 Image Upload to a New Study Use Case Description .....	13
	38.4.2.2 Use Case #2: Image Upload to an Existing Study.....	13
85	38.4.2.2.1 Image Upload to an Existing Study Use Case Description .....	13
	38.4.2.2.2 Image Upload to an Existing Study Process Flow.....	14
	38.5 WIC Security Considerations.....	15
	38.6 WIC Cross Profile Considerations.....	15
	<b>Volume 2 – Transactions .....</b>	<b>17</b>
90	4.108 Store Instances over the Web [RAD-108] .....	17
	4.108.1 Scope .....	17
	4.108.2 Actor Roles.....	17
	4.108.3 Referenced Standards .....	17
	4.108.4 Messages .....	18
95	4.108.4.1 Store Instances Message.....	18
	4.108.4.1.1 Trigger Events .....	18
	4.108.4.1.2 Message Semantics.....	18

	4.108.4.1.2.1 Capture Device Attribute Requirements.....	19
	4.108.4.1.2.2 Lightweight Modality Attribute Requirements.....	20
100	4.108.4.1.2.3 Single-frame Image.....	20
	4.108.4.1.2.3.1 JPEG Storage Option .....	21
	4.108.4.1.2.3.2 PNG Storage Option .....	21
	4.108.4.1.2.4 Multi-frame Video .....	22
	4.108.4.1.2.4.1 MPEG4 Storage Option .....	22
105	4.108.4.1.2.5 Evidence Document Storage Option.....	22
	4.108.4.1.2.6 DICOM Instance Storage Option.....	24
	4.108.4.1.3 Expected Actions .....	24
	4.108.4.1.3.1 PNG Storage Option .....	24
	4.108.4.2 Return Status Message .....	25
110	4.108.4.2.1 Trigger Events .....	25
	4.108.4.2.2 Message Semantics.....	25
	4.108.4.2.3 Expected Actions .....	25
	4.108.5 Security Considerations.....	25
	4.108.5.1 Security Audit Considerations.....	25
115	4.108.5.2 Transport Security .....	25
	<b>Volume 3 – Cross-Transaction Specifications.....</b>	<b>26</b>

## Introduction to this Supplement

- 120 There is an increasing use of mobile devices such as smartphones or tablets for image capture or viewing in healthcare. For example, a clinician can use a tablet to launch an image viewer via the EMR. The camera on the mobile device can capture high quality still images and videos. However, there is no standard way for these devices to upload captured images or evidence documents directly to the Image Manager.
- 125 The Web-based Image Capture (WIC) Profile provides a simple, lightweight, mobile-friendly mechanism to encode and send captured images, videos and evidence documents from the mobile device to the Image Manager so that these objects can be easily integrated into the rest of the imaging workflow.
- 130 The Encounter-based Imaging Workflow (EBIW) Profile complements WIC and provides a more comprehensive solution to handle image acquisition on smartphones, cameras, etc. Readers of WIC are highly encouraged to also read EBIW.

## Open Issues and Questions

No open issues.

## Closed Issues

1	<p>Should the Receiver be required to convert QuickTime (.mov) into MPEG-4 (.mp4)? iOS can only create QuickTime video encoded as H.264 video stream. QuickTime is not a DICOM supported video container format.</p> <p>Ans: Closed. Named option in Image Manager.</p>
2	<p>Should the Receiver be required to convert .3GP into MPEG-4?</p> <p>Other devices (e.g., Blackberry) use .3GP container for its MPEG-4 encoded video stream. It is used in older version of mobile SDKs, but newer version supports MP4 container directly.</p> <p>Ans: Closed. Named option in Image Manager.</p>
3	<p>Should the Receiver be required to convert PNG into lossless JPEG (.70)</p> <p>Most mobile SDK supports creation of images using JPEG (lossy) or PNG (lossless). JPEG is compatible with DICOM while PNG is not.</p> <p>Ans: Closed. Named option in Image Manager.</p>
4	<p>Should a Receiver be added that doesn't have to convert to binary instances?</p> <p>Ans: No. The Receiver must support returning binary instances upon request.</p>

5	<p>Should each media type be a separate transaction?</p> <p>Currently there is only one transaction and each media type is a named option.</p> <p>Ans: Keep one transaction.</p>
6	<p>Do we need to add H.265 video?</p> <p>Newer mobile SDK (e.g., iOS 8) supports creating video encoded in H.265 which is not yet supported by DICOM.</p> <p>Ans: Closed. Do not support H.265 encoding now. Feedback is still welcome.</p>
7	<p>Are specific details needed for the AVC / H.264 video bit stream to be compatible with the DICOM Transfer Syntax?</p> <p>Ans: Closed. WIC does not specify any more specific details other than the use of AVC/H.264. Feedback is still welcome.</p>
8	<p>Should there be more specific details about the PNG encoding?</p> <p>Ans: Closed. Added 8-bit per channel.</p>
9	<p>Should WIC also support audio or waveform capture?</p> <p>Ans: Closed. No suitable SOP Class in DICOM for general audio capture. If business case exists, then perhaps a new encapsulated audio IOD can be introduced. Feedback is still welcome.</p>
10	<p>Should the different contents be named options or defer to product documents?</p> <p>Ans: Closed. Named option.</p>
11	<p>For evidence document with bulk data, should the media type of the payload be generic application/octet-stream or more specific application/pdf for PDF and text/xml for CDA?</p> <p>Currently STOW-RS expects using the generic octet-stream.</p> <p>Ans: Specific for PDF and CDA. Submit CP to DICOM WG-27.</p>
12	<p>Should support for encapsulated PDF and CDA be in scope or not?</p> <p>Ans: In scope.</p>
13	<p>What should the Receiver use in the response message body (JSON or XML)?</p> <p>Currently STOW-RS allows either XML or JSON in the response message body.</p> <p>The Receiver should honor the HTTP Accept field.</p> <p>What if it accepts both? Match what was used in the Request?</p> <p>Ask WG-27 about 6.6.1.3. Intention is to stay compatible with STOW-RS</p> <p>Ans: Closed. Add note in Expected Action on Receiver to honor HTTP Accept field.</p>

135 **IHE Technical Frameworks General Introduction**

The [IHE Technical Framework General Introduction](#) is shared by all of the IHE domain technical frameworks. Each technical framework volume contains links to this document where appropriate.

**9 Copyright Licenses**

140 IHE technical documents refer to, and make use of, a number of standards developed and published by several standards development organizations. Please refer to the IHE Technical Frameworks General Introduction, [Chapter 9 - Copyright Licenses](#) for copyright license information for frequently referenced base standards. Information pertaining to the use of IHE International copyrighted materials is also available there.

145 **10 Trademark**

IHE® and the IHE logo are trademarks of the Healthcare Information Management Systems Society in the United States and trademarks of IHE Europe in the European Community. Please refer to the IHE Technical Frameworks General Introduction, [Chapter 10 - Trademark](#) for information on their use.

150

## IHE Technical Frameworks General Introduction Appendices

The [IHE Technical Framework General Introduction Appendices](#) are components shared by all of the IHE domain technical frameworks. Each technical framework volume contains links to these documents where appropriate.

155

*Update the following appendices to the General Introduction as indicated below. Note that these are **not** appendices to this domain's Technical Framework (TF-1, TF-2, TF-3 or TF-4) but rather, they are appendices to the IHE Technical Frameworks General Introduction located [here](#).*

160

### [Appendix A](#) – Actors

*Add the following **new or modified** actors to the [IHE Technical Frameworks General Introduction Appendix A](#):*

165

New (or modified) Actor Name	Definition
Image Capturer	A creator of DICOM composite instances.

The table below lists *existing* actors that are utilized in this profile.

#### Complete List of Existing Actors Utilized in this Profile

Existing Actor Name	Definition
Image Manager	Stores DICOM objects without guarantee of long-term storage.

170

### [Appendix B](#) – Transactions

*Add the following **new or modified** transactions to the [IHE Technical Frameworks General Introduction Appendix B](#):*



New (or modified) Transaction Name and Number	Definition
Store Instances over the Web [RAD-108]	<p>This transaction is used by the Sender to send well-formed DICOM composite objects in either DICOM binary format, or in metadata and bulk data format to the Receiver for storage.</p> <p>The instances may be images, video, DICOM evidence documents (such as Key Image Notes, or Presentation States) or binary DICOM objects. Typically, the instances will have been newly created by the Sender. The instances may be sent as part of an existing DICOM Study, or part of a new Study.</p>

175

## Appendix D – Glossary

Add the following *new or modified* glossary terms to the [IHE Technical Frameworks General Introduction Appendix D](#):

180

Glossary Term	Definition
No new terms	

185

# Volume 1 – Profiles

## 38 Web-based Image Capture (WIC) Profile


190 There is an increasing use of mobile devices such as smartphones or tablets for image capture or  
viewing in healthcare. For example, a clinician can use a tablet to launch an image viewer via the  
EMR. The camera on the mobile device can capture high quality still images and videos.  
195 However, there is no standard way for these devices to upload captured images or evidence  
documents directly to the Image Manager.

The Web-based Image Capture (WIC) Profile provides a simple, lightweight, mobile-friendly  
195 mechanism to encode and send captured images, videos and evidence documents from the  
mobile device to the Image Manager so that these objects can be easily integrated into the rest of  
the imaging workflow.

### 38.1 WIC Actors, Transactions, and Content Modules

This section defines the actors, transactions, and/or content modules in this profile. General  
200 definitions of actors are given in the Technical Frameworks General Introduction Appendix A at  
[http://ihe.net/Technical\\_Frameworks](http://ihe.net/Technical_Frameworks).

Figure 38.1-1 shows the actors directly involved in the WIC Profile and the relevant transactions  
between them. If needed for context, other actors that may be indirectly involved due to their  
205 participation in other related profiles are shown in dotted lines. Actors which have a mandatory  
grouping are shown in conjoined boxes.

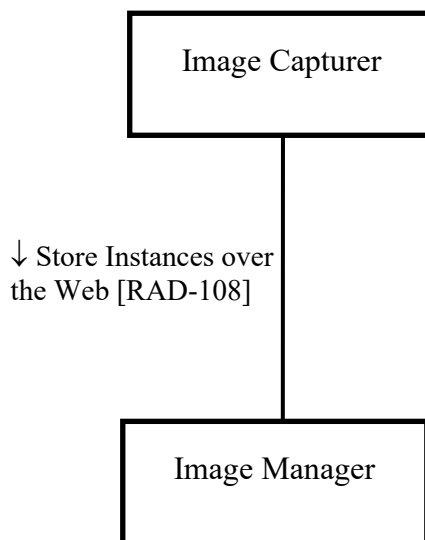

**Figure 38.1-1: WIC Actor Diagram**

210 Table 38.1-1 lists the transactions for each actor directly involved in the WIC Profile. To claim compliance with this profile, an actor shall support all required transactions (labeled “R”) and may support the optional transactions (labeled “O”).

**Table 38.1-1: WIC Profile - Actors and Transactions**

Actors	Transactions	Optionality	TF Reference
Image Capturer	Store Instances over the Web [RAD-108]	R	RAD TF-2: 4.108.1
Image Manager	Store Instances over the Web [RAD-108]	R	RAD TF-2: 4.108.1

### 38.1.1 Actor Descriptions and Actor Profile Requirements

215 Most requirements are documented in Transactions (Volume 2 and 3). This section documents any additional requirements on this profile’s actors.

#### 38.1.1.1 Image Manager

The Image Manager shall support JPEG, MPEG4, DICOM Instance and Evidence Document Storage.

### 38.2 WIC Actor Options

220 Options that may be selected for each actor in this profile, if any, are listed in the Table 38.2-1. Dependencies between options when applicable are specified in notes.

**Table 38.2-1: WIC - Actors and Options**

Actor	Option Name	TF Reference
Image Capturer (Note 1)	JPEG Storage	Section 38.2.1
	MPEG4 Storage	Section 38.2.2
	Evidence Document Storage	Section 38.2.3
	DICOM Instance Storage	Section 38.2.4
	PNG Storage	Section 38.2.5
Image Manager (Note 2)	PNG Storage	Section 38.2.5

Note 1: The Image Capturer shall support at least one option.

Note 2: The Image Manager is required to support JPEG, MPEG4, DICOM Instance and Evidence Document Storage.

225

#### 38.2.1 JPEG Storage Option

The Image Capturer captures still images in baseline JPEG format (i.e., DICOM Transfer Syntax 1.2.840.10008.1.2.4.50) and stores to the Image Manager using the DICOM PS3.18 metadata and bulk data. See RAD TF-2: 4.108.4.1.2.3.1.

230 **38.2.2 MPEG4 Storage Option**

The Image Capturer captures video stream encoded in AVC/H.264 format using a MP4 container and stores to the Image Manager using the DICOM PS3.18 metadata and bulk data. See RAD TF-2: 4.108.4.1.2.4.1.

**38.2.3 Evidence Document Storage Option**

235 The Image Capturer supports creation of DICOM instances using DICOM Native XML Format or JSON Metadata format for evidence documents such as GSPS, SR, KOS, and DICOM Encapsulated PDF/CDA. See RAD TF-2: 4.108.4.1.2.5.

**38.2.4 DICOM Instance Storage Option**

240 The Image Capturer supports creation or transmissions of DICOM instances encoded in DICOM binary format. See RAD TF-2: 4.108.4.1.2.6.

**38.2.5 PNG Storage Option**

The Image Capturer supports creation of images in lossless PNG format. See RAD TF-2: 4.108.4.1.2.3.2.

245 The Image Manager supports storing images in lossless PNG format and conversion of PNG images to an appropriate standard uncompressed or lossless (reversible) compressed Transfer Syntax. See RAD TF-2: 4.108.4.1.3.1.

**38.3 WIC Required Actor Groupings**

250 An actor from this profile (Column 1) shall implement all of the required transactions and/or content modules in this profile *in addition to* all of the transactions required for the grouped actor (Column 2).

Section 38.5 describes some optional groupings that may be of interest for security considerations and Section 38.6 describes some optional groupings in other related profiles.

**Table 38.3-1: WIC - Required Actor Groupings**

WIC Actor	Actor to be grouped with	Reference
Image Capturer	None	--
Image Manager	None	--

255 **38.4 WIC Overview**

**38.4.1 Concepts**

The Web-based Image Capture Profile enables an imaging-enabled client application running on a wide variety of devices (ranging from workstation to lightweight mobile devices) to transmit DICOM instances to the server using HTTP(S).

260 Instead of creating a DICOM PS3.10 binary instance, WIC supports DICOM PS3.18 which defines the Native DICOM Model in XML and a DICOM JSON Object Model. This enables non-traditional imaging clients (such as the clients might be used in wound care department, dermatology, etc.) to create proper DICOM instances using common tools like XML and JSON.

### **38.4.2 Use Cases**

#### **265 38.4.2.1 Use Case #1: Image Upload to a New Study**

##### **38.4.2.1.1 Image Upload to a New Study Use Case Description**

**Clinical Use Case:** A nurse in the wound care department sees patients in the ward. She photographs the wounds to track the healing process. She uses one of the department’s photo cameras, a departmental tablet or her mobile phone to take a series of pictures of a patient. She immediately imports the images in the imaging system under the correct patient name and adds an appropriate report note in the patient chart.

This use case is addressed by the Lightweight Modality in the Encounter-Based Imaging Workflow (EBIW) Profile. EBIW incorporates the Store Instances over the Web [RAD-108] transaction defined by WIC for RESTful storage of images.


#### **275 38.4.2.2 Use Case #2: Image Upload to an Existing Study**

##### **38.4.2.2.1 Image Upload to an Existing Study Use Case Description**

**Clinical Use Case:** A radiologist uses a tablet to retrieve a study from the central repository. While viewing the study, she identifies certain key images and adds some markup indicating the region of interest. Finally, she creates a report. When she saves the changes, the application sends the markups, key objects and reports to the central repository for persistent storage.

**Technical Use Case 1:** The Imaging Document Consumer retrieves and views a study from the Imaging Document Source using the Web-based Image Access (WIA) Profile. The Imaging Document Consumer, grouped with the Image Capturer, creates new evidence documents (e.g., Key Image Notes, screen captures as Secondary Capture, etc.) using the same patient and study context. The Image Capturer then uploads the created evidence documents to the Image Manager.

**38.4.2.2.2 Image Upload to an Existing Study Process Flow**

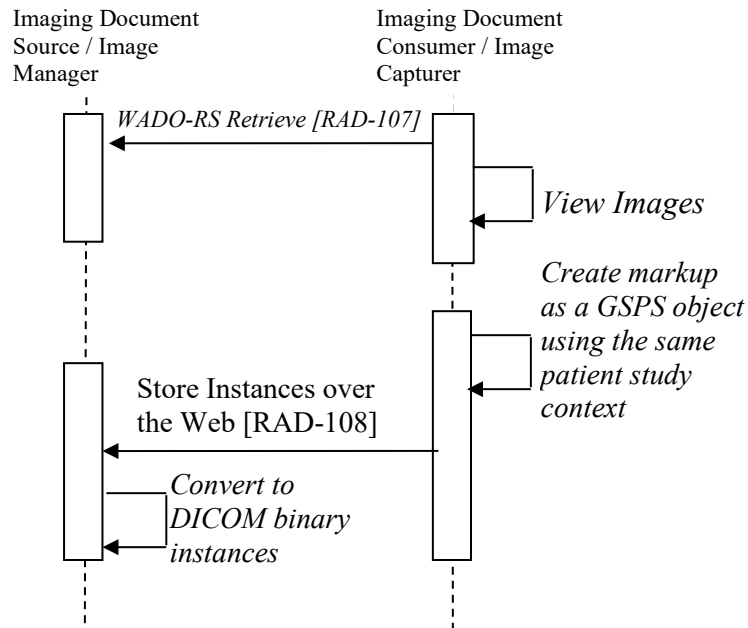

**Figure 38.4.2.2.2-1: Image Upload to an Existing Study Process Flow in WIC Profile**

290 **Technical Use Case 2:** Similarly, using the Invoke Image Display (IID) Profile, an EMR, as an Image Display Invoker, launches an Image Display to view a patient’s study. Using the markup tools and key image tools provided by the Image Display, the user creates new markups and tag certain images as key images. The IID Image Display, grouped with the Image Capturer, stores the markup and key images in the same patient and study context to the Image Manager using  
 295 DICOM JSON Object Model. The Image Manager receives the instances and converts them into DICOM binary format. Another Image Display (not part of this profile), which is a traditional PACS workstation, retrieves the study and presents the markup as well as key images.

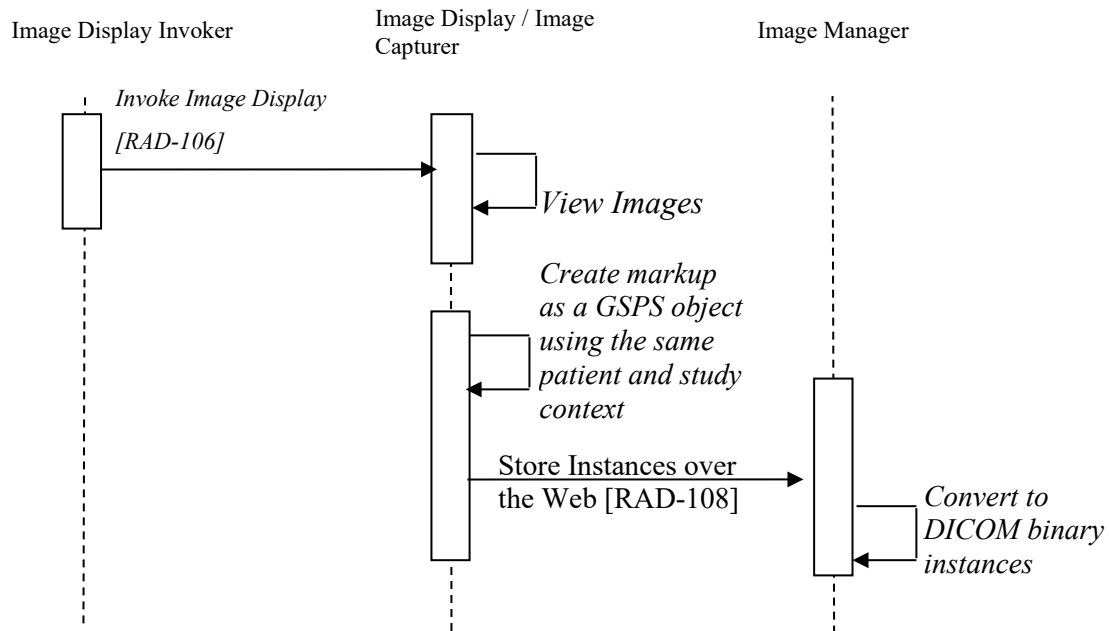


Figure 38.4.2.2-2: Image Upload to an Existing Study Process Flow in WIC Profile

300 **38.5 WIC Security Considerations**

Since the Image Capturer may be running in a mobile device outside of the hospital private network, it is important to ensure that the communication between the Image Capturer and the Image Manager is secure. Encryption specified in the ITI [Audit Trail and Node Authentication](#) (ATNA) Profile can provide secure data transport. ATNA audit messages can ensure audit trails for private health information are captured.

It is recommended that the Image Manager will be grouped with the ATNA Secure Node or Secure Application to record audit messages for the transactions performed. It is not expected that the Image Capturer will record audit messages.

310 The Image Manager may want to restrict which users are authorized to upload. The ITI [Internet User Authorization](#) (IUA) Profile provides OAuth-based user authorization.

The Image Manager may want to restrict which devices are authorized to upload. ATNA provides certificate-based node authentication.

315 Since the Image Capturer may be running in a mobile device that can easily be lost, it is important to consider how much information should be retained in the mobile device. This includes patient demographics as well as the images, videos or reports.

**38.6 WIC Cross Profile Considerations**

**IID – Invoke Image Display**

320 An Image Capturer might be grouped with an Image Display in the Invoke Image Display Profile to create and store evidence documents back to the associated Image Manager based on images being viewed and their associated patient and study context.

**XDS-I.b – Cross-Enterprise Document Sharing for Imaging**

An Image Capturer might be grouped with an XDS-I.b Imaging Document Consumer to create and store new objects back to the Image Manager based on study objects it is viewing.

325 An Image Manager might be grouped with an XDS-I.b Imaging Document Source to receive objects sent from an Image Capturer and publish a new manifest.

**WIA – Web-based Image Access**

An Image Capturer might be grouped with an WIA Imaging Document Consumer to create and store new objects back to the Image Manager based on study objects it is viewing.

330 An Image Manager might be grouped with an WIA Imaging Document Source to receive objects sent from an Image Capturer.

**ITI PDQm – Patient Demographics Query for Mobile**

An Image Capturer might be grouped with a PDQm Patient Demographics Consumer to retrieve reliable patient demographics from the Patient Demographics Supplier.



## Volume 2 – Transactions

335 *Add Section 4.108*

### 4.108 Store Instances over the Web [RAD-108]

#### 4.108.1 Scope

This transaction is used by the Sender to send well-formed DICOM composite objects in either DICOM binary format, or in metadata and bulk data format to the Receiver for storage.

340 The instances may be images, video, DICOM evidence documents (such as Key Image Notes, or Presentation States) or binary DICOM objects. Typically, the instances will have been newly created by the Sender. The instances may be sent as part of an existing DICOM Study, or part of a new Study.

#### 4.108.2 Actor Roles

345 The Roles in this transaction are defined in the following table and may be played by the actors shown here:

**Table 4.108.2-1: Actor Roles**

<b>Role:</b>	<b>Sender:</b> Creates and sends well-formed DICOM composite objects
<b>Actor(s):</b>	The following actors may play the role of Sender: Image Capturer Lightweight Modality
<b>Role:</b>	<b>Receiver:</b> Receives objects from the Sender
<b>Actor(s):</b>	The following actors may play the role of Receiver: Image Manager

350 Transaction text specifies behavior for each Role. The behavior of specific actors may also be specified when it goes beyond that of the general Role.

#### 4.108.3 Referenced Standards

DICOM [PS3.3](#): Information Object Definitions

DICOM [PS3.4](#): Service Class Specifications

DICOM [PS3.5 Section B.2](#): UUID Derived UID

355 DICOM [PS3.18 Section 10.5](#): Web Services - Store Transaction of the DICOM Studies Service


DICOM [PS3.18 Annex F](#): DICOM JSON Model

DICOM [PS3.19 Section A.1](#): Native DICOM Model

DICOM [PS3.19 Annex B](#): Interfaces Definition (WSDL and Schema)

ISO/IEC 14496-14:2003: MPEG-4 Part 14

360 **4.108.4 Messages**

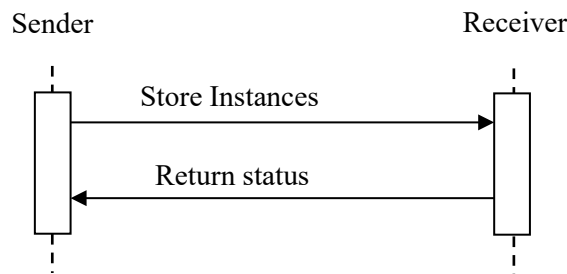

**Figure 4.108.4-1: Interaction Diagram**

**4.108.4.1 Store Instances Message**

The Sender creates one or more instances and sends these instances to the Receiver for storage.

365 There may be one or more Senders storing instances to the same Receiver at any given time.

**4.108.4.1.1 Trigger Events**

User or application initiates transfer of the acquired or created instances to the Receiver.

**4.108.4.1.2 Message Semantics**

370 The Store Instances message is a Store transaction of the DICOM Studies Service. See [DICOM PS3.18 Section 10.5](#).

The Sender is the User Agent. The Receiver is the Origin Server.

The message shall correspond to the DICOM Resource in Table 4.108.4.1.2-1.

**Table 4.108.4.1.2-1: Store Transaction DICOM Resources**

Resource	URI Template	Expected Response
Study	http://<location>/studies/{study}	All instances that belong to the same Study, i.e., each representation shall have the same Study Instance UID

375 The parameters of the message are defined in Table 4.108.4.1.2-2. All path parameter names are case-sensitive.

**Table 4.108.4.1.2-2: Store Transaction Request Parameters**

Parameter Name	Description	Notes
<location>	The host name, an optional port address, and may be followed by an optional path.	See the discussion about location in <a href="#">ITI TF-2: 3.11.4.1.2 Message Semantics</a> .
{study}	Study Instance UID of the study to be stored.	

The Sender shall encode the instances per DICOM PS3.18 Section 10.5.1.4, using either:

- the binary DICOM method
- Metadata and Bulkdata representations of SOP instances.

380

The Sender shall encode the Metadata and Bulkdata request as either:

- Array of DICOM JSON Model Object
- XML request messages as defined in the Native DICOM Model, with one message part per XML object

385

Note: STOW-RS specifies Native DICOM Model as a baseline and JSON Model Object is optional. The Sender may support either one.

If the Sender needs to create new unique identifiers (e.g., for Study Instance UID, Series Instance UID or SOP Instance UID), it shall do so using UUID Derived UID mechanism specified in DICOM [PS3.5 Section B.2](#).

390

Details about when it is appropriate to trigger the creation of a new Study/Series/SOP Instance are described in RAD TF-2: 4.8.4.1.1.1 “Study UIDs and Series UIDs”.

#### 4.108.4.1.2.1 Capture Device Attribute Requirements

A Sender that is a Capture Device (i.e., digital camera) shall populate patient demographics according to Table 4.108.4.1.2-1 in order to provide the appropriate patient context for the created DICOM Instances. Additional patient demographics can be populated by the Sender according to DICOM [PS3.3 Section C.7.1.1](#).

395

Note: The means by which the Sender obtains the existing study values to populate these attributes is not specified here but might include using another transaction, extracting them from the integrated viewer, or via the user interface provided by the Sender.

400

**Table 4.108.4.1.2-1: Critical Patient Demographics Attributes**

DICOM Attribute	Opt.	Existing Study Case (RAD TF-1: 38.4.2.2)
Patient’s Name (0010,0010)	R	Equal to existing study
Patient ID (0010,0020)	R	Equal to existing study
Issuer of Patient ID (0010,0021)	R	Equal to existing study
Patient’s Birth Date (0010,0030)	R	Equal to existing study
Patient’s Sex (0010,0040)	R	Equal to existing study

405 When sending Metadata, the Sender shall populate Type 1 study attributes and also Type 2 study attributes for which the value is known for the SOP class being stored. If a reliable source of metadata attributes is available, values from that source shall be used, e.g., the study attributes may be populated by either extracting the study attributes from the integrated viewer, or via the user interface provided by the Sender. Otherwise, the Sender shall populate study attributes according to Table 4.108.4.1.2-2. The Sender populates additional study attributes according to DICOM [PS3.3 Section C.7.2.1](#) and [C.7.3.1](#).

**Table 4.108.4.1.2-2: Critical Study Attributes**

DICOM Attribute	Opt.	Existing Study Case (RAD TF-1: 38.4.2.2)
Study Instance UID (0020,000D)	R	Equal to existing study
Accession Number (0008,0050)	R	Equal to existing study
Issuer of Accession Number Sequence (0008,0051)	R	Equal to existing study
Series Date (0008,0021)	R	Acquisition date
Series Time (0008,0031)	R	Acquisition time
Series Description (0008,103E)	R	Possibly pre-configured or user input
Performed Procedure Step ID (0040,0253)	O	Internally generated
Performed Procedure Step Start Date (0040,0244)	O	Acquisition date
Performed Procedure Step Start Time (0040,0245)	O	Acquisition time
Performed Procedure Step Description (0040,0254)	O	Possibly pre-configured, user input, or from existing study
Request Attribute Sequence (0040,0275)	R	
> Reason for Requested Procedure (0040,1002)	R	Possibly pre-configured, user input, or from existing study
> Reason for Requested Procedure Code Sequence (0040,100A)	O	Possibly pre-configured, user input, or from existing study

410

#### 4.108.4.1.2.2 Lightweight Modality Attribute Requirements

A Sender that is a Lightweight Modality in the Encounter-Based Imaging Workflow (EBIW) Profile shall populate metadata attributes as shown in Table 4.131.4.1.2-1.

#### 4.108.4.1.2.3 Single-frame Image

415 The Sender shall encode compressed single-frame image pixel data elements in one message part per instance.

The Sender shall include all required attributes in the Native DICOM Model or the DICOM JSON Model Object for the appropriate DICOM SOP Class.

420 Table 4.108.4.1.2.3-1 identifies recommended SOP Classes for commonly captured single-frame image types. DICOM defines more specific SOP Classes that may be used if applicable (see DICOM [PS3.3](#)).

**Table 4.108.4.1.2.3-1: Recommended SOP Classes for Single-frame Images**

Captured Image Type	SOP Class Name	SOP Class UID	IOD Specification defined in DICOM PS3.3
Photographs	VL Photographic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.4	VL Photographic Image IOD
Screenshots	Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	Secondary Capture Image IOD

425 According to DICOM [PS3.18 Section 10.5.1.4](#), the Image Pixel Description Macro attributes may be omitted. This exception is driven by the inability of certain mobile SDK or mobile clients (e.g., zero footprint browser client) to obtain the image pixel information.

**Table 4.108.4.1.2.3-2: Image Pixel Description Macro Attributes**

Attribute Name	Tag
Samples per Pixel	(0028,0002)
Photometric Interpretation	(0028,0004)
Rows	(0028,0010)
Columns	(0028,0011)
Bits Allocated	(0028,0100)
Bits Stored	(0028,0101)
High Bit	(0028,0102)
Pixel Representation	(0028,0103)

#### 4.108.4.1.2.3.1 JPEG Storage Option

430 A Sender that supports the JPEG Storage Option shall be capable of sending images that are created using JPEG compression.

If the Sender knows the Transfer Syntax of the JPEG image, the Sender shall encode the compressed pixel data using single-frame Media Types described in DICOM [PS3.18 Section 8.7.3.1](#).

435 If the Sender does not know the Transfer Syntax of the JPEG image, the Sender shall use a media type of `image/jpeg`.

#### 4.108.4.1.2.3.2 PNG Storage Option

A Sender that claims the PNG Storage Option shall be capable of creating images using lossless PNG compression with 8-bit per channel.

The Sender shall use a media type of `image/png`.

440 **4.108.4.1.2.4 Multi-frame Video**

The Sender shall encode compressed multi-frame video pixel data elements in one message part per instance.

The Sender shall include all required attributes in the Native DICOM Model or DICOM JSON Model Object for the appropriate DICOM SOP Class.

445 Table 4.108.4.1.2.4-1 identifies recommended SOP Classes for commonly captured multi-frame video types. DICOM defines more specific SOP Classes that may be used if applicable (see DICOM [PS3.3](#)).

**Table 4.108.4.1.2.4-1: Recommended SOP Classes for Multi-frame Videos**

Captured Video Type	SOP Class Name	SOP Class UID	IOD Specification defined in DICOM PS3.3
Video Photographs	Video Photographic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.4.1	Video Photographic Image IOD

450 According to DICOM [PS3.18 Section 10.5.1.4](#), the Image Pixel Description Macro attributes may be omitted; see Table 4.108.4.1.2.3-2. This exception is driven by the inability of certain mobile SDK or mobile clients (e.g., zero footprint browser client) to obtain the image pixel information.

**4.108.4.1.2.4.1 MPEG4 Storage Option**

455 A Sender that supports the MPEG4 Storage Option shall be capable of sending videos that are encoded using AVC/H.264.

If the Sender knows the Transfer Syntax of the created video, the Sender shall encode the compressed video stream using a Media Type described in [DICOM PS3.18 Section 8.7.3.1](#).

460 If the Sender does not know the Transfer Syntax of the created video and the created video is using an MPEG4 container, then the Sender shall use a media type of `video/mp4`.

The Sender shall support at least the `video/mp4` media type. When using the `video/mp4` media type, the MPEG-4 video stream shall be encoded using the AVC/H.264 encoding scheme and stored in the MP4 container format (ISO/IEC 14496-14:2003).

**4.108.4.1.2.5 Evidence Document Storage Option**

465 The Sender shall encode the complete evidence document metadata in the first part of the multipart request.

The Sender shall include all required attributes in the Native DICOM Model or the DICOM JSON Model Object for the appropriate DICOM SOP Class that is used for the evidence document.

470 Table 4.108.4.1.2.5-1 identifies recommended SOP Classes for commonly created evidence documents. DICOM defines more specific SOP Classes that may be used if applicable (see [DICOM PS3.3](#)).

**Table 4.108.4.1.2.5-1: Recommended SOP Classes for Evidence Document**

Captured Evidence Document Type	SOP Class Name	SOP Class UID	IOD Specification defined in DICOM PS3.3
Presentation State	Grayscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.1	Grayscale Softcopy Presentation State IOD
	Color Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.2	Color Softcopy Presentation State IOD
	Pseudo-Color Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.3	Pseudo-color Softcopy Presentation State IOD
Structured Report	Basic Text SR	1.2.840.10008.5.1.4.1.1.88.11	Basic Text SR IOD
	Enhanced SR	1.2.840.10008.5.1.4.1.1.88.22	Enhanced SR IOD
	Comprehensive SR	1.2.840.10008.5.1.4.1.1.88.33	Comprehensive SR IOD
	Comprehensive 3D SR	1.2.840.10008.5.1.4.1.1.88.34	Comprehensive 3D SR IOD
Key Object Selection	Key Object Selection Document	1.2.840.10008.5.1.4.1.1.88.59	Key Object Selection Document IOD
Encapsulated Document	Encapsulated PDF Storage	1.2.840.10008.5.1.4.1.1.104.1	Encapsulated PDF IOD
	Encapsulated CDA Storage	1.2.840.10008.5.1.4.1.1.104.2	Encapsulated CDA IOD

475 The Sender shall include each encapsulated document in its own separate message part in the DICOM Request Message Body with the following HTTP headers:

- Encapsulated PDF document
  - Content-Type: application/pdf
  - Content-Location: {BulkDataURI}
- 480 • Encapsulated CDA document
  - Content-Type: text/xml
  - Content-Location: {BulkDataURI}
- Other encapsulated document
  - Content-Type: application/octet-stream
  - 485 • Content-Location: {BulkDataURI}

The expected endpoint for DICOM Encapsulated PDF / CDA documents is a DICOM server.

Note: For transmission of plain PDF or CDA documents that are not intended to be DICOM encapsulated and stored to a DICOM server, the ITI [Mobile Access to Health Documents](#) (MHD) Profile provides a more appropriate mechanism for uploading electronic health records.

490 **4.108.4.1.2.6 DICOM Instance Storage Option**

The Sender shall encode each DICOM instance as a separate message part.

The Sender shall send the DICOM instances using DICOM binary format.

**4.108.4.1.3 Expected Actions**

The Receiver shall accept and process the message payload.

495 The Receiver shall accept Metadata and Bulkdata encoded in either the Native DICOM Model or DICOM JSON Model Object.

The Receiver shall at least support the SOP Classes defined in Tables 4.108.4.1.2.3-1, 4.108.4.1.2.4-1 and 4.108.4.1.2.5-1.

500 If the message contents are not binary DICOM instances, the Receiver shall convert the DICOM Metadata and Bulkdata into DICOM binary instances according to the SOP Class UID specified in the metadata.

If the received object includes empty Image Pixel Macro Attributes (see Table 4.108.4.1.2-1), the Receiver shall populate them according to the Image Pixel Attribute Descriptions specified in DICOM [PS3.3 Section C.7.6.3.1](#).

505 The Receiver shall store the DICOM binary instances (either received or converted) such that they can be later queried or retrieved in a fashion meeting the requirements defined for a DICOM Level 2 Storage SCP (refer to DICOM [PS3.4 Section B.4.1](#)).

510 If the received object includes the Transfer Syntax in the media type parameter, then the Receiver shall use the same Transfer Syntax when converting the Metadata and Bulkdata into DICOM binary instances.

If the media type of the received object is `image/jpeg`, then the Receiver shall use the Transfer Syntax 1.2.840.10008.1.2.4.50 when converting the Metadata and Bulkdata into DICOM binary instances.

515 If the media type of the received object is `video/mpeg2` or `video/mp4`, then the Receiver shall use the appropriate Transfer Syntax for the received object as defined in DICOM [PS3.18](#), Table 8.7.3-5.

**4.108.4.1.3.1 PNG Storage Option**

520 A Receiver that supports the PNG Storage Option shall convert the encoded lossless PNG image into DICOM binary format with an appropriate standard uncompressed or lossless (reversible) compressed Transfer Syntax.

**Table 4.108.4.1.3.1-1: Eligible Transfer Syntaxes for PNG Storage**

Media Type	Eligible Transfer Syntax	Description
image/png	1.2.840.10008.1.2	Implicit VR Little Endian: Default Transfer Syntax for DICOM
	1.2.840.10008.1.2.1	Explicit VR Little Endian



Media Type	Eligible Transfer Syntax	Description
	1.2.840.10008.1.2.1.99	Deflated Explicit VR Little Endian
	1.2.840.10008.1.2.4.57	JPEG Lossless, Non-Hierarchical (Process 14)
	1.2.840.10008.1.2.4.70	JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 [Selection Value 1]): Default Transfer Syntax for Lossless JPEG Image Compression
	1.2.840.10008.1.2.4.80	JPEG-LS Lossless Image Compression
	1.2.840.10008.1.2.4.90	JPEG 2000 Image Compression (Lossless Only)
	1.2.840.10008.1.2.4.92	JPEG 2000 Part 2 Multi-component Image Compression (Lossless Only)
	1.2.840.10008.1.2.5	RLE Lossless

#### 4.108.4.2 Return Status Message

The Receiver reports the outcome of the Store Instances Message.

##### 525 4.108.4.2.1 Trigger Events

The Receiver receives a Store Instances Message.

##### 4.108.4.2.2 Message Semantics

The Receiver shall return a response to the Sender according to DICOM [PS3.18 Section 10.5.3](#).

The Sender is the User Agent. The Receiver is the Origin Server.

530 Note: The Receiver may return a response before all processing is complete for the received object; for example, performing required image conversion asynchronously after sending the response. Sender implementers should be aware that such post-response processing may fail.

Note: The Receiver will honor the HTTP Accept header field for encoding of the response message. However, if the Sender accepts both XML and JSON, then the Receiver can choose either format for the response message.

##### 535 4.108.4.2.3 Expected Actions

The Sender has no expected actions.

#### 4.108.5 Security Considerations

##### 4.108.5.1 Security Audit Considerations

540 The [Radiology Audit Trail Option](#) in the IHE ITI [Audit Trail and Node Authentication](#) (ATNA) Profile ([ITI TF-1:9](#)) defines audit requirements for IHE Radiology transactions. See RAD TF-3: 5.1.1.

##### 4.108.5.2 Transport Security

In order to avoid unauthorized interception of private health information, the communication over HTTP may be secured by using HTTPS.

545

## Volume 3 – Cross-Transaction Specifications

*Update Volume 3, Table 5.1-2 to add a new row for RAD-108. Note that transactions are listed in numeric order.*

550

**Table 5.1-2: IHE Radiology transactions and resulting ATNA trigger events**

IHE Radiology Transaction	ATNA Trigger Event(s)	Actor(s) that shall be able to record audit event
Patient Registration [RAD-1]	Patient-record-event	ADT Order Placer, DSS/OF - when PHI is presented
...		
<b><u>Store Instances over the Web [RAD-108]</u></b>	<b><u>Instances-stored</u></b>	<b><u>Receiver: Image Manager</u></b>
...		